

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Time of Inspection: 11:19

Date of Inspection: 11/23/2020

Serial Number: 80-004587

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#: 201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#: 201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 1190213 Exp: 08/28/2022
0.000	0.050	0.081	0.199	0.080
0.000	0.049	0.081	0.200	0.079
0.000	0.049	0.080	0.200	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Charles Owen McConnell Gayle

Signature and Printed Name

CHARLES OWEN MCCONNELL GAYLE

11/23/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Time of Inspection: 14:16

Date of Inspection: 10/20/2020

Serial Number: 80-004587

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.049	0.083	0.198	0.080
0.000	0.049	0.083	0.200	0.079
0.000	0.049	0.083	0.200	0.079

Number of Simulators Used: 4


Remarks:

POWER FAILURE DURING TEST HAD TO REDO INSPECTION

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.





CHARLES OWEN MCCONNELL GAYLE

Signature and Printed Name

10/20/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 10:20

Date of Inspection: 09/01/2020

Serial Number: 80-004587
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.048	0.079	0.197	0.079
0.000	0.049	0.079	0.197	0.078
0.000	0.049	0.080	0.199	0.077

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Charles E McConnell Charles E McConnell
Signature and Printed Name

09/01/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

016321

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Serial Number: 80-004587

Time of Inspection: 15:44

Date of Inspection: 08/03/2020

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.048	0.079	0.198	0.080
0.000	0.048	0.079	0.199	0.080
0.000	0.048	0.079	0.199	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Daniel E Lyons
DANIEL E LYONS

Signature and Printed Name

08/03/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT – INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Time of Inspection: 17:42

Date of Inspection: 07/14/2020

Serial Number: 80-004587

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.049	0.079	0.197	0.080
0.000	0.049	0.079	0.199	0.080
0.000	0.049	0.079	0.199	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

07/14/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Time of Inspection: 20:42

Date of Inspection: 07/06/2020

Serial Number: 80-004587

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.049	0.079	0.197	0.080
0.000	0.049	0.080	0.199	0.079
0.000	0.049	0.081	0.198	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

07/06/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 14:48

Date of Inspection: 06/22/2020

Serial Number: 80-004587
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.049	0.080	0.198	0.080
0.000	0.050	0.080	0.199	0.080
0.000	0.049	0.080	0.199	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

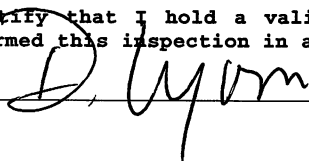

DANIEL E LYONS

Signature and Printed Name

06/22/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: **OSCEOLA COUNTY S.O.**

Time of Inspection: **12:43**

Date of Inspection: **02/26/2020**

Serial Number: **80-004587**

Software: **8100.27**

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:_____ Exp:_____	0.20g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:_____ Exp:_____
/ 0.000	INT / INT			
/ 0.000				
/ 0.000				

Number of Simulators Used: 5

Remarks:

00: Ambient Fail. 05: Interferent Detect, Interferent Detect. Non-compliance: .

The above instrument complies () does not comply (☒) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

DANIEL E LYONS

Signature and Printed Name

02/26/2020
Date

Kirkland, Brett

From: Dan Lyons <dlyo@OSCEOLA.ORG>
Sent: Wednesday, February 26, 2020 5:04 PM
To: Platt, Shayla; 'McKnight, Jamie (JMcknight@sao9.org)'; 'SherryForcier@flhsmv.gov'; 'Atkinson, Karsona'; 'orlandobar@flhsmv.gov'; Brian Adams; Michael Hernandez; Alcohol Testing Program
Subject: 26 Feb monthly inspections
Attachments: 26 Feb 2020 Monthly Intox Inspec.pdf

ALCON,

I received instrument 80-005935 back on 02/25/2020 from FDLE with the Annual Inspection completed on 02/04/2020. I received instrument 80-003935 back on 02/26/2020 from CMI. FDLE completed the Annual Inspection on 02/21/2020.

The monthly Agency Inspection Report was conducted 02/26/2020 on the following instruments; 80-000966, 80-000968, 80-001715, 80-003935, 80-003937, 80-004587 and 80-005935.

Ref to instrument 80-004587, the Alcohol Free Test, Received and Ambient Fail. The instrument was re-tested. The re-test results were within standards. In reference to the 0.05g/210L Test, I received and interferent detected. I re-tested and received the same error. I did attempt to contact FDLE for guidance with negative results. I removed the instrument from service.

In reference to 80-000968, 80-003937 and 80-004587, have been sent out to FDLE for the annual inspection.

All intox inspections are complete and with the exception of 80-004587, all are in compliance with 11D-8.

Thank you

V/R

Attention: The information contained in this E-mail message is privileged and confidential information intended only for the use of the individual(s) named above. If the reader of this message is not the intended recipient, you are hereby notified that any dissemination, distribution or copy of this communication is strictly prohibited. If you have received this communication in error, please contact the sender by reply E-mail and destroy all copies of the original message.

Florida Department of Law Enforcement Alcohol Testing Program

80-004587
TSK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 18:16

Date of Inspection: 02/07/2020

Serial Number: 80-004587
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2020
0.000	0.052	0.080	0.198	0.080
0.000	0.052	0.079	0.199	0.080
0.000	0.052	0.080	0.199	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

02/07/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

80-004587
BK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 14:55

Date of Inspection: 01/24/2020

Serial Number: 80-004587
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.051	0.078	0.193	0.078
0.000	0.051	0.078	0.195	0.078
0.000	0.051	0.078	0.197	0.078

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

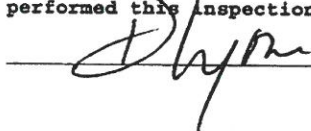

Signature and Printed Name

DANIEL E LYONS

01/24/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

80-004587
BK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Time of Inspection: 12:02

Date of Inspection: 01/03/2020

Serial Number: 80-004587

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.052	0.079	0.197	0.079
0.000	0.051	0.079	0.197	0.079
0.000	0.051	0.079	0.198	0.078

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

01/03/2020
Date