



INSTRUMENT PROCESSING SHEET

Agency Brevard CSO

S/N 80-000940

Florida Department of
Law Enforcement

Date In 08/04/2020 DI Completion Date 08/06/2020

☒ Ship ☐ P/U ☐ H/D ☐ CMI ☐ EE

Intake Performed By <u>TDG</u> ☒ Annual ☐ Registration ☐ Return from CMI / EE Visual Inspection: ☒ Case ☒ Handle ☐ Keyboard ☒ Dry Gas Shelf ☒ Feet ☒ Breath Tube ☒ Ports ☒ Screws Tight Other Equipment/ Accessories: ☒ Power cord ☐ Printer Cable ☒ Static Bag ☐ 12V DC Cable Notes: <u>Instrument came w/out keyboard.</u>	Quality Checks Performed By <u>TDG</u> ☒ Breath Tube Screen ☒ Replace External O-Rings ☒ Instrument Set Up Verified ☒ R-Value <u>135</u> ☒ Flow Verification (L/s) Flow Column # <u>ATP106</u> 32 mm <u>0.144</u> (.139 - .169) 36 mm <u>0.156</u> (.156 - .190) 53 mm <u>0.234</u> (.228 - .278) 103 mm <u>0.496</u> (.447 - .547) ☒ Barometric Pressure Check Gauge ID # <u>68639</u> ☒ Stability Checks <table border="1" style="width:100%; border-collapse: collapse;"> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #/Exp</th> </tr> <tr> <td>0.050</td> <td>SD3967</td> <td>201905A 05/14/2021</td> </tr> <tr> <td>0.080</td> <td>SD3968</td> <td>201905B 05/14/2021</td> </tr> <tr> <td>0.200</td> <td>SD3969</td> <td>201904D 04/30/2021</td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td>AG003005 01/30/2022</td> </tr> </table>	Simulator	Serial #	Lot #/Exp	0.050	SD3967	201905A 05/14/2021	0.080	SD3968	201905B 05/14/2021	0.200	SD3969	201904D 04/30/2021	0.080 DGS	N/A	AG003005 01/30/2022	Flow Calibration Performed By _____ Flow Column # _____ ☐ 5L/min - 17mm ☐ 15L/min - 53mm ☐ 30L/min - 103mm ☐ R-Value _____ ☐ Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547)																																													
Simulator	Serial #	Lot #/Exp																																																												
0.050	SD3967	201905A 05/14/2021																																																												
0.080	SD3968	201905B 05/14/2021																																																												
0.200	SD3969	201904D 04/30/2021																																																												
0.080 DGS	N/A	AG003005 01/30/2022																																																												
Final Release Date FDLE Alcohol Testing Program Digitally signed by FDLE Alcohol Testing Program Date: 2020.08.07 16:23:06 -04'00'	Maintenance Performed By _____ ☐ Battery Replacement ☐ Dry Gas Regulator Replacement ☐ Breath Tube Replacement ☐ Other _____ Temperature Checks Performed By <u>MH</u> ☒ Lab Temp °C <u>22.75</u> External Digital Therm. ID#: <u>300504</u> ☒ 34°C +- .2 Serial #: <u>MP4863</u> ☒ 34°C +- .2 Serial #: <u>MP4864</u> ☒ 34°C +- .2 Serial #: <u>MP5097</u>																																																													
Calibration Adjustment Performed By <u>MH</u> Barometric Pressure Gauge <u>1016</u> ID # <u>28199</u> <table border="1" style="width:100%; border-collapse: collapse;"> <tr> <th>Simulator</th> <th>Serial Number</th> <th>Lot Number</th> <th>Expiration</th> </tr> <tr> <td>0.000</td> <td>MP5095</td> <td>N/A</td> <td>N/A</td> </tr> <tr> <td>0.040</td> <td>MP5098</td> <td>20060</td> <td>02/10/2022</td> </tr> <tr> <td>0.100</td> <td>MP5099</td> <td>20190</td> <td>04/06/2022</td> </tr> <tr> <td>0.200</td> <td>MP5100</td> <td>20160</td> <td>03/18/2022</td> </tr> <tr> <td>0.300</td> <td>MP5101</td> <td>20030</td> <td>01/21/2022</td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td>08819080A1</td> <td>06/05/2021</td> </tr> </table> ☒ Post Calibration Adjustment Stability Checks <table border="1" style="width:100%; border-collapse: collapse;"> <tr> <th>Simulator</th> <th>Serial Number</th> <th>Lot Number</th> <th>Expiration</th> </tr> <tr> <td>0.050</td> <td>MP4863</td> <td>201905A</td> <td>05/14/2021</td> </tr> <tr> <td>0.080</td> <td>MP4864</td> <td>201905B</td> <td>05/14/2021</td> </tr> <tr> <td>0.200</td> <td>MP5097</td> <td>201904D</td> <td>04/30/2021</td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td>AG003005</td> <td>01/30/2022</td> </tr> </table>	Simulator	Serial Number	Lot Number	Expiration	0.000	MP5095	N/A	N/A	0.040	MP5098	20060	02/10/2022	0.100	MP5099	20190	04/06/2022	0.200	MP5100	20160	03/18/2022	0.300	MP5101	20030	01/21/2022	0.080 DGS	N/A	08819080A1	06/05/2021	Simulator	Serial Number	Lot Number	Expiration	0.050	MP4863	201905A	05/14/2021	0.080	MP4864	201905B	05/14/2021	0.200	MP5097	201904D	04/30/2021	0.080 DGS	N/A	AG003005	01/30/2022	Department Inspection Performed By <u>MH</u> Barometric Pressure ID# <u>28663</u> Gauge <u>1016</u> Instrument <u>1016</u> Mouth Alcohol Solution Lot # <u>2020-A</u> Acetone Stock Solution Lot # <u>2019-A</u> <table border="1" style="width:100%; border-collapse: collapse;"> <tr> <th>Simulator</th> <th>Serial Number</th> </tr> <tr> <td>0.000</td> <td>SD1014</td> </tr> <tr> <td>Interferent</td> <td>SD1015</td> </tr> <tr> <td>0.050</td> <td>MP4863</td> </tr> <tr> <td>0.080</td> <td>MP4864</td> </tr> <tr> <td>0.200</td> <td>MP5097</td> </tr> </table>		Simulator	Serial Number	0.000	SD1014	Interferent	SD1015	0.050	MP4863	0.080	MP4864	0.200	MP5097
Simulator	Serial Number	Lot Number	Expiration																																																											
0.000	MP5095	N/A	N/A																																																											
0.040	MP5098	20060	02/10/2022																																																											
0.100	MP5099	20190	04/06/2022																																																											
0.200	MP5100	20160	03/18/2022																																																											
0.300	MP5101	20030	01/21/2022																																																											
0.080 DGS	N/A	08819080A1	06/05/2021																																																											
Simulator	Serial Number	Lot Number	Expiration																																																											
0.050	MP4863	201905A	05/14/2021																																																											
0.080	MP4864	201905B	05/14/2021																																																											
0.200	MP5097	201904D	04/30/2021																																																											
0.080 DGS	N/A	AG003005	01/30/2022																																																											
Simulator	Serial Number																																																													
0.000	SD1014																																																													
Interferent	SD1015																																																													
0.050	MP4863																																																													
0.080	MP4864																																																													
0.200	MP5097																																																													
Notes/Suggested Service: _____ _____ _____ _____ _____ _____	Attachments ☒ Form 41 ☒ Stability Checks ☒ Calibration Certificate ☒ Calibration Adjustment ☒ Post-Stability Checks ☐ Flow Calibration ☒ Form 40 ☐ Other _____ ☒ Instrument Complies with Chapter 11D-8, FAC ☐ Instrument Does Not Comply with Chapter 11D-8, FAC ☒ Return to/Place into Evidentiary Use ☐ Remain Out of Evidentiary Use ☒ Conduct an Agency Inspection Before Evidentiary Use David Eliezer Reyes Rivera Digitally signed by David Eliezer Reyes Rivera Date: 2020.08.06 15:09:33 -04'00' <u>Brett Kirkland</u> 2020.08.07 16:14:47 -04'00' Tech Review / Date Admin Review / Date																																																													

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: BREVARD COUNTY S.O.
Time of Inspection: 11:49

Date of Inspection: 08/06/2020

Serial Number: 80-000940
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201905A Exp: 05/14/2021	0.08g/210L Test (g/210L) Lot#:201905B Exp: 05/14/2021	0.20g/210L Test (g/210L) Lot#:201904D Exp: 04/30/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG003005 Exp: 01/30/2022
0.000	0.048	0.079	0.199	0.079
0.000	0.049	0.078	0.199	0.079
0.000	0.049	0.079	0.199	0.078
0.000	0.048	0.078	0.200	0.078
0.000	0.049	0.078	0.200	0.078
0.000	0.049	0.078	0.199	0.078
0.000	0.049	0.078	0.200	0.078
0.000	0.049	0.079	0.199	0.078
0.000	0.049	0.079	0.199	0.077
0.000	0.049	0.078	0.200	0.077


Standard Deviations	0.0004	0.0005	0.0005	0.0006
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0005 Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MICHAEL D HAUGHEY

Signature and Printed Name

08/06/2020
Date

DERR Digitally signed
by DERR
Date: 2020.08.06
15:08:45 -04'00'

TYPE OF TEST	SERIAL NUMBER	AGENCY	DATE	PERFORMED BY
Stabilities - Post	80-000940	Brevard County SO	08/06/2020	MX

0.05g/210L	0.08g/210L	0.20g/210L	DGS 0.08g/210L
0.047 to 0.053 ☒	0.077 to 0.083 ☒	0.194 to 0.206 ☒	0.077 to 0.083 ☒

BREVARD COUNTY S.O.
Intoxilyzer - Alcohol Analyzer
Model 8000
08/06/2020
Software: 8100.27

BREVARD COUNTY S.O.
Intoxilyzer - Alcohol Analyzer
Model 8000
08/06/2020
Software: 8100.27

BREVARD COUNTY S.O.
Intoxilyzer - Alcohol Analyzer
Model 8000
08/06/2020
Software: 8100.27

BREVARD COUNTY S.O.
Intoxilyzer - Alcohol Analyzer
Model 8000
08/06/2020
Software: 8100.27

Test g/210L Time

Air Blank 0.000 09:56

Control Test 0.049 09:57

Air Blank 0.000 09:57

Control Test 0.049 09:58

Air Blank 0.000 09:59

Control Test 0.049 09:59

Air Blank 0.000 10:00

Control Test Stats

Average 0.0490

Std Dev 0.0000

Rel Std Dev(%) 0.0000

Test g/210L Time

Air Blank 0.000 10:01

Control Test 0.079 10:02

Air Blank 0.000 10:02

Control Test 0.078 10:03

Air Blank 0.000 10:03

Control Test 0.078 10:04

Air Blank 0.000 10:05

Control Test Stats

Average 0.0783

Std Dev 0.0006

Rel Std Dev(%) 0.7370

Test g/210L Time

Air Blank 0.000 10:06

Control Test 0.199 10:06

Air Blank 0.000 10:07

Control Test 0.199 10:08

Air Blank 0.000 10:08

Control Test 0.198 10:09

Air Blank 0.000 10:10

Control Test Stats

Average 0.1987

Std Dev 0.0006

Rel Std Dev(%) 0.2906

Test g/210L Time

Air Blank 0.000 10:11

Control Test 0.080 10:11

Air Blank 0.000 10:12

Control Test 0.079 10:12

Air Blank 0.000 10:12

Control Test 0.080 10:13

Air Blank 0.000 10:13

Control Test Stats

Average 0.0797

Std Dev 0.0006

Rel Std Dev(%) 0.7247

Operator's Signature

MX

Operator's Signature

MX

Operator's Signature

MX

Operator's Signature

MX



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
4700 Terminal Drive, Suite 1
Ft. Myers, FL 33907

This is to certify the calibration of Intoxilyzer 8000 serial number 80-000940, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-000940</u>	UNCERTAINTY* $\pm$	
Owning Agency:	<u>BREVARD COUNTY S.O.</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>08/06/2020</u>	0.080 g/ 210 L	0.005
Calibration Time:	<u>11:49</u>	0.200 g/ 210 L	0.007
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.
*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ($k=3$).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Thermometer temperatures are checked with NIST traceable Eutechnics 4400 digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the uses of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards.
This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

Digitally signed
by DERR
Date: 2020.08.06
15:07:10 -0400



08/06/2020

Date

MICHAEL D HAUGHEY,
Department Inspector

2020.08.07
16:17:56
-0400

BK

FDLE/ATP Form 69 April 2020

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality

BREWARD COUNTY S.O.
Intoxilyzer - Alcohol Analyzer
Model 8000
08/06/2020 09:17:01
SN 80-000940
Auto Calibration
Max Power Res Value = 41
Auto Range Res Value = 27

Sol Value = 0.000 g/210L ***
Fit Value = 0.0000 mg/l %
Samples Taken = 4, Discarded = 1
Sum Io = 12831, Sum Io = 12521
***** CHANNEL 1 *****
Sample % Abs (% Abs Ref)
Sample #1 = 0.2160 (-0.0220)
Sample #2 = 0.1900 (-0.0170)
Sample #3 = 0.1950 (-0.0210)
Sample #4 = 0.1800 (-0.0160)
Avg % Abs = 0.1863 (-0.0330)
STD DEV = 0.0055 (-0.0243)
REL STD DEV = 2.956 (73.730)

***** CHANNEL 2 *****
Sample % Abs (% Abs Ref)
Sample #1 = 0.2470 (-0.0110)
Sample #2 = 0.2340 (-0.0100)
Sample #3 = 0.2060 (-0.0250)
Sample #4 = 0.2100 (-0.0370)
Avg % Abs = 0.2167 (-0.0240)
STD DEV = 0.0151 (-0.0135)
REL STD DEV = 6.989 (56.366)

Sol Value = 0.040 g/210L ***
Fit Value = 0.1905 mg/l %
Samples Taken = 4, Discarded = 1
Sum Io = 12820, Sum Io = 12516
***** CHANNEL 1 *****
Sample % Abs (% Abs Ref)
Sample #1 = 0.9530 (-0.0200)
Sample #2 = 0.9470 (-0.0270)
Sample #3 = 0.9620 (-0.0020)
Sample #4 = 0.9750 (-0.0160)
Avg % Abs = 0.9613 (-0.0137)
STD DEV = 0.0140 (-0.0146)
REL STD DEV = 1.458 (107.123)

***** CHANNEL 2 *****
Sample % Abs (% Abs Ref)
Sample #1 = 1.7030 (-0.0080)
Sample #2 = 1.6830 (-0.0200)
Sample #3 = 1.6780 (-0.0310)
Sample #4 = 1.7030 (-0.0060)
Avg % Abs = 1.6880 (-0.0130)
STD DEV = 0.0132 (-0.0157)
REL STD DEV = 0.784 (120.894)

Sol Value = 0.100 g/210L ***
Fit Value = 0.4762 mg/l %
Samples Taken = 4, Discarded = 1
Sum Io = 12818, Sum Io = 12514
***** CHANNEL 1 *****
Sample % Abs (% Abs Ref)
Sample #1 = 2.1000 (-0.0170)
Sample #2 = 2.0820 (-0.0080)
Sample #3 = 2.0860 (-0.0030)
Sample #4 = 2.0670 (-0.0160)
Avg % Abs = 2.0783 (-0.0070)
STD DEV = 0.0100 (-0.0095)
REL STD DEV = 0.482 (136.277)

***** CHANNEL 2 *****
Sample % Abs (% Abs Ref)
Sample #1 = 3.8290 (-0.0000)
Sample #2 = 3.8050 (-0.0220)
Sample #3 = 3.8070 (-0.0250)
Sample #4 = 3.8160 (-0.0270)
Avg % Abs = 3.8093 (-0.0247)
STD DEV = 0.0059 (-0.0025)
REL STD DEV = 0.154 (110.202)

Sol Value = 0.200 g/210L ***
Fit Value = 0.9524 mg/l %
Samples Taken = 4, Discarded = 1
Sum Io = 12820, Sum Io = 12513
***** CHANNEL 1 *****
Sample % Abs (% Abs Ref)
Sample #1 = 3.9730 (-0.0190)
Sample #2 = 3.9220 (-0.0170)
Sample #3 = 3.9250 (-0.0420)
Sample #4 = 3.9020 (-0.0310)
Avg % Abs = 3.9163 (-0.0300)
STD DEV = 0.0125 (-0.0125)
REL STD DEV = 0.319 (41.767)

***** CHANNEL 2 *****
Sample % Abs (% Abs Ref)
Sample #1 = 7.2660 (-0.0180)
Sample #2 = 7.2060 (-0.0340)
Sample #3 = 7.1820 (-0.0520)
Sample #4 = 7.1880 (-0.0460)
Avg % Abs = 7.1920 (-0.0440)
STD DEV = 0.0125 (-0.0092)
REL STD DEV = 0.174 (20.830)

Sol Value = 0.300 g/210L ***
Fit Value = 1.4286 mg/l %
Samples Taken = 4, Discarded = 1
Sum Io = 12814, Sum Io = 12508
***** CHANNEL 1 *****
Sample % Abs (% Abs Ref)
Sample #1 = 5.6780 (-0.0240)
Sample #2 = 5.6500 (-0.0140)
Sample #3 = 5.6500 (-0.0070)
Sample #4 = 5.6500 (-0.0090)
Avg % Abs = 5.6500 (-0.0050)
STD DEV = 0.0000 (-0.0108)
REL STD DEV = 0.000 (216.333)

***** CHANNEL 2 *****
Sample % Abs (% Abs Ref)
Sample #1 = 10.3600 (-0.0100)
Sample #2 = 10.2990 (-0.0220)
Sample #3 = 10.3110 (-0.0420)
Sample #4 = 10.3130 (-0.0260)
Avg % Abs = 10.3077 (-0.0300)
STD DEV = 0.0076 (-0.0106)
REL STD DEV = 0.073 (35.277)

80-000940
08/06/2020
Cal Adj.

MX

***** AUTO CAL DATA *****
***** CHANNEL 1 *****
Sol Val = 0.0000 mg/l or 0.000 g/210L
% Abs = 0.186
Std Dev = 0.01 Rel Std Dev = 2.96
Sol Val = 0.1905 mg/l or 0.040 g/210L
% Abs = 0.961
Std Dev = 0.01 Rel Std Dev = 1.46
Sol Val = 0.4762 mg/l or 0.100 g/210L
% Abs = 2.078
Std Dev = 0.01 Rel Std Dev = 0.48
Sol Val = 0.9524 mg/l or 0.200 g/210L
% Abs = 3.916
Std Dev = 0.01 Rel Std Dev = 0.32
Sol Val = 1.4286 mg/l or 0.300 g/210L
% Abs = 5.650
Std Dev = 0.00 Rel Std Dev = 0.00
Zero Order Coef = -451.67
First Order Coef = 2430.82
Second Order Coef = 31.18
Standard Deviation = 18.61633

***** CHANNEL 2 *****
Sol Val = 0.0000 mg/l or 0.000 g/210L
% Abs = 0.217
Std Dev = 0.02 Rel Std Dev = 6.99
Sol Val = 0.1905 mg/l or 0.040 g/210L
% Abs = 1.688
Std Dev = 0.01 Rel Std Dev = 0.78
Sol Val = 0.4762 mg/l or 0.100 g/210L
% Abs = 3.809
Std Dev = 0.01 Rel Std Dev = 0.15
Sol Val = 0.9524 mg/l or 0.200 g/210L
% Abs = 7.192
Std Dev = 0.01 Rel Std Dev = 0.17
Sol Val = 1.4286 mg/l or 0.300 g/210L
% Abs = 10.308
Std Dev = 0.01 Rel Std Dev = 0.07
Zero Order Coef = -264.00
First Order Coef = 1257.31
Second Order Coef = 14.87
Standard Deviation = 17.267677

Solution Stats Quadratic Fit Chan 1
Act Fit Residual
g/210L g/210L g/210L
0.000 0.000 -0.0000
0.040 0.040 -0.0002
0.100 0.099 0.0006
0.200 0.200 -0.0005
0.300 0.300 0.0002

Solution Stats Quadratic Fit Chan 2
Act Fit Residual
g/210L g/210L g/210L
0.000 0.000 -0.0002
0.040 0.040 0.0001
0.100 0.100 0.0004
0.200 0.201 -0.0005
0.300 0.300 0.0002

Sol Value = 0.080 g/210L ***
Fit Value = 0.3810 mg/l %
Samples Taken = 4, Discarded = 1
***** CHANNEL 1 *****
Sample #1 = 2802.00
Sample #2 = 2789.00
Sample #3 = 2845.00
Sample #4 = 2753.00
Average Result = 2795.6667
STD DEV = 46.3609
REL STD DEV = 1.658

***** CHANNEL 2 *****
Sample #1 = 3111.00
Sample #2 = 3088.00
Sample #3 = 3115.00
Sample #4 = 3107.00
Average Result = 3103.3333
STD DEV = 13.8684
REL STD DEV = 0.447




Dry Gas H2O Adjust Results *****
Barometric Pressure = 1016
3 um H2O Adjust (mg/l x 10,000) = 1014
9 um H2O Adjust (mg/l x 10,000) = 706
***** AUTO CAL PASS *****

Digitally signed
by DERR
Date: 2020.08.06
15:06:22 -0400

2020.08.07
16:19:01 -0400

BK

TYPE OF TEST	SERIAL NUMBER	AGENCY	DATE	PERFORMED BY
Stabilities	80-000940	Brevard CSD	08/05/2020	TMG

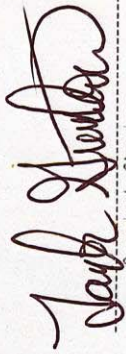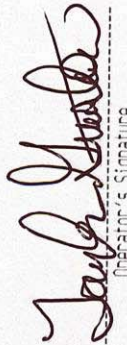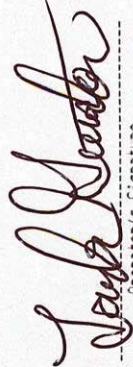0.05g/210L 0.047 to 0.053 ☒	0.08g/210L 0.077 to 0.083 ☒	0.20g/210L 0.194 to 0.206 ☒	DGS 0.08g/210L 0.077 to 0.083 ☒																																																																																																																																																
BREVARD COUNTY S.O. Intoxilyzer - Alcohol Analyzer Model 8000 08/05/2020 Software: 8100.27 <table><thead><tr><th>Test</th><th>g/210L</th><th>Time</th></tr></thead><tbody><tr><td>Air Blank</td><td>0.000</td><td>13:12</td></tr><tr><td>Control Test</td><td>0.052</td><td>13:13</td></tr><tr><td>Air Blank</td><td>0.000</td><td>13:14</td></tr><tr><td>Control Test</td><td>0.051</td><td>13:14</td></tr><tr><td>Air Blank</td><td>0.000</td><td>13:15</td></tr><tr><td>Control Test</td><td>0.050</td><td>13:15</td></tr><tr><td>Air Blank</td><td>0.000</td><td>13:16</td></tr><tr><td>Control Test Stats</td><td></td><td></td></tr><tr><td>Average</td><td>0.0510</td><td></td></tr><tr><td>Std Dev</td><td>0.0010</td><td></td></tr><tr><td>Rel Std Dev(%)</td><td>1.9608</td><td></td></tr></tbody></table> Operator's Signature 	Test	g/210L	Time	Air Blank	0.000	13:12	Control Test	0.052	13:13	Air Blank	0.000	13:14	Control Test	0.051	13:14	Air Blank	0.000	13:15	Control Test	0.050	13:15	Air Blank	0.000	13:16	Control Test Stats			Average	0.0510		Std Dev	0.0010		Rel Std Dev(%)	1.9608		BREVARD COUNTY S.O. Intoxilyzer - Alcohol Analyzer Model 8000 08/05/2020 Software: 8100.27 <table><thead><tr><th>Test</th><th>g/210L</th><th>Time</th></tr></thead><tbody><tr><td>Air Blank</td><td>0.000</td><td>13:17</td></tr><tr><td>Control Test</td><td>0.081</td><td>13:18</td></tr><tr><td>Air Blank</td><td>0.000</td><td>13:18</td></tr><tr><td>Control Test</td><td>0.080</td><td>13:19</td></tr><tr><td>Air Blank</td><td>0.000</td><td>13:20</td></tr><tr><td>Control Test</td><td>0.081</td><td>13:20</td></tr><tr><td>Air Blank</td><td>0.000</td><td>13:21</td></tr><tr><td>Control Test Stats</td><td></td><td></td></tr><tr><td>Average</td><td>0.0807</td><td></td></tr><tr><td>Std Dev</td><td>0.0006</td><td></td></tr><tr><td>Rel Std Dev(%)</td><td>0.7157</td><td></td></tr></tbody></table> Operator's Signature 	Test	g/210L	Time	Air Blank	0.000	13:17	Control Test	0.081	13:18	Air Blank	0.000	13:18	Control Test	0.080	13:19	Air Blank	0.000	13:20	Control Test	0.081	13:20	Air Blank	0.000	13:21	Control Test Stats			Average	0.0807		Std Dev	0.0006		Rel Std Dev(%)	0.7157		BREVARD COUNTY S.O. Intoxilyzer - Alcohol Analyzer Model 8000 08/05/2020 Software: 8100.27 <table><thead><tr><th>Test</th><th>g/210L</th><th>Time</th></tr></thead><tbody><tr><td>Air Blank</td><td>0.000</td><td>13:22</td></tr><tr><td>Control Test</td><td>0.200</td><td>13:23</td></tr><tr><td>Air Blank</td><td>0.000</td><td>13:23</td></tr><tr><td>Control Test</td><td>0.200</td><td>13:24</td></tr><tr><td>Air Blank</td><td>0.000</td><td>13:25</td></tr><tr><td>Control Test</td><td>0.200</td><td>13:25</td></tr><tr><td>Air Blank</td><td>0.000</td><td>13:26</td></tr><tr><td>Control Test Stats</td><td></td><td></td></tr><tr><td>Average</td><td>0.2000</td><td></td></tr><tr><td>Std Dev</td><td>0.0000</td><td></td></tr><tr><td>Rel Std Dev(%)</td><td>0.0000</td><td></td></tr></tbody></table> Operator's Signature 	Test	g/210L	Time	Air Blank	0.000	13:22	Control Test	0.200	13:23	Air Blank	0.000	13:23	Control Test	0.200	13:24	Air Blank	0.000	13:25	Control Test	0.200	13:25	Air Blank	0.000	13:26	Control Test Stats			Average	0.2000		Std Dev	0.0000		Rel Std Dev(%)	0.0000		BREVARD COUNTY S.O. Intoxilyzer - Alcohol Analyzer Model 8000 08/05/2020 Software: 8100.27 <table><thead><tr><th>Test</th><th>g/210L</th><th>Time</th></tr></thead><tbody><tr><td>Air Blank</td><td>0.000</td><td>13:27</td></tr><tr><td>Control Test</td><td>0.076</td><td>13:28</td></tr><tr><td>Air Blank</td><td>0.000</td><td>13:28</td></tr><tr><td>Control Test</td><td>0.077</td><td>13:29</td></tr><tr><td>Air Blank</td><td>0.000</td><td>13:29</td></tr><tr><td>Control Test</td><td>0.077</td><td>13:29</td></tr><tr><td>Air Blank</td><td>0.000</td><td>13:29</td></tr><tr><td>Control Test Stats</td><td></td><td></td></tr><tr><td>Average</td><td>0.0767</td><td></td></tr><tr><td>Std Dev</td><td>0.0006</td><td></td></tr><tr><td>Rel Std Dev(%)</td><td>0.7531</td><td></td></tr></tbody></table> Operator's Signature 	Test	g/210L	Time	Air Blank	0.000	13:27	Control Test	0.076	13:28	Air Blank	0.000	13:28	Control Test	0.077	13:29	Air Blank	0.000	13:29	Control Test	0.077	13:29	Air Blank	0.000	13:29	Control Test Stats			Average	0.0767		Std Dev	0.0006		Rel Std Dev(%)	0.7531	
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	13:12																																																																																																																																																	
Control Test	0.052	13:13																																																																																																																																																	
Air Blank	0.000	13:14																																																																																																																																																	
Control Test	0.051	13:14																																																																																																																																																	
Air Blank	0.000	13:15																																																																																																																																																	
Control Test	0.050	13:15																																																																																																																																																	
Air Blank	0.000	13:16																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0510																																																																																																																																																		
Std Dev	0.0010																																																																																																																																																		
Rel Std Dev(%)	1.9608																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	13:17																																																																																																																																																	
Control Test	0.081	13:18																																																																																																																																																	
Air Blank	0.000	13:18																																																																																																																																																	
Control Test	0.080	13:19																																																																																																																																																	
Air Blank	0.000	13:20																																																																																																																																																	
Control Test	0.081	13:20																																																																																																																																																	
Air Blank	0.000	13:21																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0807																																																																																																																																																		
Std Dev	0.0006																																																																																																																																																		
Rel Std Dev(%)	0.7157																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	13:22																																																																																																																																																	
Control Test	0.200	13:23																																																																																																																																																	
Air Blank	0.000	13:23																																																																																																																																																	
Control Test	0.200	13:24																																																																																																																																																	
Air Blank	0.000	13:25																																																																																																																																																	
Control Test	0.200	13:25																																																																																																																																																	
Air Blank	0.000	13:26																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.2000																																																																																																																																																		
Std Dev	0.0000																																																																																																																																																		
Rel Std Dev(%)	0.0000																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	13:27																																																																																																																																																	
Control Test	0.076	13:28																																																																																																																																																	
Air Blank	0.000	13:28																																																																																																																																																	
Control Test	0.077	13:29																																																																																																																																																	
Air Blank	0.000	13:29																																																																																																																																																	
Control Test	0.077	13:29																																																																																																																																																	
Air Blank	0.000	13:29																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0767																																																																																																																																																		
Std Dev	0.0006																																																																																																																																																		
Rel Std Dev(%)	0.7531																																																																																																																																																		

Failed stabilities. Needs optical calibration. TMG 8/5/2020

DERR
Digitally signed
by DERR
Date: 2020.08.06
15:04:18 -04'00'

2020.08.07
162003
-04'00'
BK

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: BREVARD COUNTY S.O.

Serial Number: 80-000940

Time of Inspection: 12:51

Date of Inspection: 08/05/2020

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08g/210L Test (g/210L) Lot#:_____ Exp:_____	0.20g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08 g/210L Dry Gas Std Test (g/210L) Lot #:_____ Exp:_____


Number of Simulators Used: _____

Remarks:

BYPASSED AI. COMPLIANCE NOT DETERMINED.

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



TAYLOR D GUTSCHOW

Signature and Printed Name

08/05/2020

Date

DERR

Digitally signed by
DERR
Date: 2020.08.06
15:03:34 -04'00'

Forgot to print before upload. MX