



INSTRUMENT PROCESSING SHEET

Agency Fort Walton Beach Police Department S/N 80-006931

Florida Department of Law Enforcement

Date In 12/11/2020 DI Completion Date 12-14-2020 Ship P/U H/D CMI EE

Intake Performed By RAW Quality Checks Performed By IS Flow Calibration Performed By Maintenance Performed By

Final Release Date FDLE Alcohol Testing Program Digitally signed by FDLE Alcohol Testing Program Date: 2020.12.18 10:32:07 -05'00'

Calibration Adjustment Performed By Barometric Pressure Gauge ID # Simulator Serial Number Lot Number Expiration

Department Inspection Performed By IS Barometric Pressure ID# 30793 Gauge 1013 Instrument 1014 Mouth Alcohol Solution Lot # 2020-A Acetone Stock Solution Lot # 2019-A

Notes/Suggested Service:

Attachments Form 41 Stability Checks Calibration Certificate Calibration Adjustment Post-Stability Checks Flow Calibration Form 40 Other Instrument Complies with Chapter 11D-8, FAC

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: FT WALTON BEACH PD
Time of Inspection: 15:26

Date of Inspection: 12/14/2020

Serial Number: 80-006931
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201905A Exp: 05/14/2021	0.08g/210L Test (g/210L) Lot#:202010B Exp: 10/05/2022	0.20g/210L Test (g/210L) Lot#:201904D Exp: 04/30/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG011102 Exp: 04/20/2022
0.000	0.048	0.078	0.200	0.080
0.000	0.048	0.078	0.200	0.080
0.000	0.048	0.079	0.200	0.080
0.000	0.048	0.079	0.200	0.080
0.000	0.048	0.079	0.200	0.080
0.000	0.048	0.079	0.200	0.079
0.000	0.048	0.079	0.200	0.079
0.000	0.048	0.079	0.200	0.079
0.000	0.048	0.079	0.200	0.079
0.000	0.048	0.079	0.200	0.079
0.000	0.048	0.079	0.200	0.079
Standard Deviations	0.0000	0.0004	0.0000	0.0005

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0002 Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.


I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Israel Soto

ISRAEL SOTO

Signature and Printed Name

12/14/2020
Date


 2020.1
 2.18
 10:31:14
 -05'00'

Stability checks

FT WALTON BEACH PD
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006931
 12/11/2020
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	15:47
Control Test	0.049	15:48
Air Blank	0.000	15:49
Control Test	0.048	15:49
Air Blank	0.000	15:50
Control Test	0.048	15:51
Air Blank	0.000	15:51
Control Test Stats		
Average	0.0483	
Std Dev	0.0006	
Rel Std Dev(%)	1.1945	

FT WALTON BEACH PD
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006931
 12/11/2020
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	15:52
Control Test	0.080	15:53
Air Blank	0.000	15:53
Control Test	0.079	15:54
Air Blank	0.000	15:55
Control Test	0.079	15:55
Air Blank	0.000	15:56
Control Test Stats		
Average	0.0793	
Std Dev	0.0006	
Rel Std Dev(%)	0.7277	

FT WALTON BEACH PD
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006931
 12/11/2020
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	15:57
Control Test	0.200	15:57
Air Blank	0.000	15:58
Control Test	0.199	15:59
Air Blank	0.000	15:59
Control Test	0.199	16:00
Air Blank	0.000	16:01
Control Test Stats		
Average	0.1993	
Std Dev	0.0006	
Rel Std Dev(%)	0.2896	

wet



Operator's Signature



Operator's Signature



Operator's Signature

FT WALTON BEACH PD
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006931
 12/11/2020
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	16:02
Control Test	0.081	16:03
Air Blank	0.000	16:03
Control Test	0.081	16:04
Air Blank	0.000	16:04
Control Test	0.081	16:05
Air Blank	0.000	16:05
Control Test Stats		
Average	0.0810	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	


Dry



Operator's Signature

MX

SR

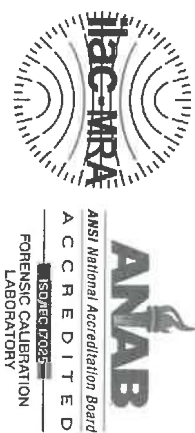

Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
2729 Fort Knox Blvd.
Bldg. 2, Suite 1300
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-006931, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-006931</u>	UNCERTAINTY* ±	
Owning Agency:	<u>FT WALTON BEACH PD</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>12/14/2020</u>	0.080 g/ 210 L	0.005
Calibration Time:	<u>15:26</u>	0.200 g/ 210 L	0.007
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/210 L. Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration. *Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence (k=3). The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/IEC 17025 Standards. Simulator temperatures are traceable to NIST. Thermometer temperatures are checked with NIST traceable Eutechnics 4400 digital thermometers calibrated by Precision Metrology in accordance with ISO/IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the uses of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/IEC 17025 standards. This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

Date 12/14/2020
Israel Soto
ISRAEL SOTO,
Department Inspector

Service • Integrity • Respect • Quality

FDLE/ATP Form 69 April 2020
Issuing Authority: Alcohol Testing Program

2020.12.18 10:29:45 -05'00'




INSTRUMENT PROCESSING SHEET

Agency Fort Walton Beach Police DepartmentS/N 80-006931

Florida Department of Law Enforcement

Date In 04/03/2020DI Completion Date 4/9/20 Ship P/U H/D CMI EE

Intake Performed By <u>RAW</u> <input checked="" type="checkbox"/> Annual <input type="checkbox"/> Registration <input checked="" type="checkbox"/> Return from CMI / EE Visual Inspection: <input checked="" type="checkbox"/> Case <input checked="" type="checkbox"/> Handle <input checked="" type="checkbox"/> Keyboard <input checked="" type="checkbox"/> Dry Gas Shelf <input checked="" type="checkbox"/> Feet <input checked="" type="checkbox"/> Breath Tube <input checked="" type="checkbox"/> Ports <input checked="" type="checkbox"/> Screws Tight Other Equipment/ Accessories: <input checked="" type="checkbox"/> Power cord <input type="checkbox"/> Printer Cable <input checked="" type="checkbox"/> Static Bag <input type="checkbox"/> 12V DC Cable Notes: _____ _____ _____	Quality Checks Performed By <u>JD</u> <input checked="" type="checkbox"/> Breath Tube Screen <input checked="" type="checkbox"/> Replace External O-Rings <input checked="" type="checkbox"/> Instrument Set Up Verified <input checked="" type="checkbox"/> R-Value <u>130</u> <input checked="" type="checkbox"/> Flow Verification (L/s) Flow Column # <u>ATP-102</u> 32 mm <u>0.152</u> (.139 - .169) 36 mm <u>0.167</u> (.156 - .190) 53 mm <u>0.238</u> (.228 - .278) 103 mm <u>0.496</u> (.447 - .547) <input checked="" type="checkbox"/> Barometric Pressure Check Gauge ID # <u>26932</u> <input checked="" type="checkbox"/> Stability Checks <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #/Exp</th> </tr> </thead> <tbody> <tr> <td>0.050</td> <td><u>MP5088</u></td> <td><u>201905A</u> <u>05-14-2021</u></td> </tr> <tr> <td>0.080</td> <td><u>MP5089</u></td> <td><u>201905B</u> <u>05-14-2021</u></td> </tr> <tr> <td>0.200</td> <td><u>MP5090</u></td> <td><u>201904D</u> <u>04-30-2021</u></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td><u>AG931603</u> <u>11-12-2021</u></td> </tr> </tbody> </table>	Simulator	Serial #	Lot #/Exp	0.050	<u>MP5088</u>	<u>201905A</u> <u>05-14-2021</u>	0.080	<u>MP5089</u>	<u>201905B</u> <u>05-14-2021</u>	0.200	<u>MP5090</u>	<u>201904D</u> <u>04-30-2021</u>	0.080 DGS	N/A	<u>AG931603</u> <u>11-12-2021</u>	Flow Calibration Performed By _____ Flow Column # _____ <input type="checkbox"/> 5L/min - 17mm <input type="checkbox"/> 15L/min - 53mm <input type="checkbox"/> 30L/min - 103mm <input type="checkbox"/> R-Value _____ <input type="checkbox"/> Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547) Maintenance Performed By _____ <input type="checkbox"/> Battery Replacement <input type="checkbox"/> Dry Gas Regulator Replacement <input type="checkbox"/> Breath Tube Replacement <input type="checkbox"/> Other _____ Temperature Checks Performed By <u>SP</u> <input checked="" type="checkbox"/> Lab Temp °C <u>21.14</u> External Digital Therm. ID#: <u>300502</u> <input checked="" type="checkbox"/> 34°C +/-2 Serial #: <u>MP5088</u> <input checked="" type="checkbox"/> 34°C +/-2 Serial #: <u>MP5089</u> <input checked="" type="checkbox"/> 34°C +/-2 Serial #: <u>MP5090</u>																																	
Simulator	Serial #	Lot #/Exp																																																
0.050	<u>MP5088</u>	<u>201905A</u> <u>05-14-2021</u>																																																
0.080	<u>MP5089</u>	<u>201905B</u> <u>05-14-2021</u>																																																
0.200	<u>MP5090</u>	<u>201904D</u> <u>04-30-2021</u>																																																
0.080 DGS	N/A	<u>AG931603</u> <u>11-12-2021</u>																																																
Final Release Date FDLE Alcohol Testing Program Digitally signed by FDLE Alcohol Testing Program Date: 2020.04.17 09:01:37 -04'00'	Calibration Adjustment Performed By <u>SP</u> Barometric Pressure Gauge <u>1013</u> ID # <u>28421</u> <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> <th>Lot Number</th> <th>Expiration</th> </tr> </thead> <tbody> <tr> <td>0.000</td> <td><u>MP5086</u></td> <td>N/A</td> <td>N/A</td> </tr> <tr> <td>0.040</td> <td><u>MP5082</u></td> <td><u>19080</u></td> <td><u>3-4-21</u></td> </tr> <tr> <td>0.100</td> <td><u>MP5083</u></td> <td><u>19160</u></td> <td><u>7-9-21</u></td> </tr> <tr> <td>0.200</td> <td><u>MP5084</u></td> <td><u>19040</u></td> <td><u>1-29-21</u></td> </tr> <tr> <td>0.300</td> <td><u>MP5085</u></td> <td><u>19010</u></td> <td><u>1-3-21</u></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td><u>03519080A4</u></td> <td><u>4-5-21</u></td> </tr> </tbody> </table> <input checked="" type="checkbox"/> Post Calibration Adjustment Stability Checks <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> <th>Lot Number</th> <th>Expiration</th> </tr> </thead> <tbody> <tr> <td>0.050</td> <td><u>MP5088</u></td> <td><u>201905A</u></td> <td><u>5-14-21</u></td> </tr> <tr> <td>0.080</td> <td><u>MP5089</u></td> <td><u>201905B</u></td> <td><u>5-14-21</u></td> </tr> <tr> <td>0.200</td> <td><u>MP5090</u></td> <td><u>201904D</u></td> <td><u>4-30-21</u></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td><u>AG931603</u></td> <td><u>11-12-21</u></td> </tr> </tbody> </table>		Simulator	Serial Number	Lot Number	Expiration	0.000	<u>MP5086</u>	N/A	N/A	0.040	<u>MP5082</u>	<u>19080</u>	<u>3-4-21</u>	0.100	<u>MP5083</u>	<u>19160</u>	<u>7-9-21</u>	0.200	<u>MP5084</u>	<u>19040</u>	<u>1-29-21</u>	0.300	<u>MP5085</u>	<u>19010</u>	<u>1-3-21</u>	0.080 DGS	N/A	<u>03519080A4</u>	<u>4-5-21</u>	Simulator	Serial Number	Lot Number	Expiration	0.050	<u>MP5088</u>	<u>201905A</u>	<u>5-14-21</u>	0.080	<u>MP5089</u>	<u>201905B</u>	<u>5-14-21</u>	0.200	<u>MP5090</u>	<u>201904D</u>	<u>4-30-21</u>	0.080 DGS	N/A	<u>AG931603</u>	<u>11-12-21</u>
Simulator	Serial Number	Lot Number	Expiration																																															
0.000	<u>MP5086</u>	N/A	N/A																																															
0.040	<u>MP5082</u>	<u>19080</u>	<u>3-4-21</u>																																															
0.100	<u>MP5083</u>	<u>19160</u>	<u>7-9-21</u>																																															
0.200	<u>MP5084</u>	<u>19040</u>	<u>1-29-21</u>																																															
0.300	<u>MP5085</u>	<u>19010</u>	<u>1-3-21</u>																																															
0.080 DGS	N/A	<u>03519080A4</u>	<u>4-5-21</u>																																															
Simulator	Serial Number	Lot Number	Expiration																																															
0.050	<u>MP5088</u>	<u>201905A</u>	<u>5-14-21</u>																																															
0.080	<u>MP5089</u>	<u>201905B</u>	<u>5-14-21</u>																																															
0.200	<u>MP5090</u>	<u>201904D</u>	<u>4-30-21</u>																																															
0.080 DGS	N/A	<u>AG931603</u>	<u>11-12-21</u>																																															
Notes/Suggested Service: _____ _____ _____ _____ _____	Department Inspection Performed By <u>SP</u> Barometric Pressure ID# <u>30793</u> Gauge <u>1008</u> Instrument <u>1010</u> Mouth Alcohol Solution Lot # <u>2019-B</u> Acetone Stock Solution Lot # <u>2019-A</u> <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> </tr> </thead> <tbody> <tr> <td>0.000</td> <td><u>MP5091</u></td> </tr> <tr> <td>Interferent</td> <td><u>MP5087</u></td> </tr> <tr> <td>0.050</td> <td><u>MP5088</u></td> </tr> <tr> <td>0.080</td> <td><u>MP5089</u></td> </tr> <tr> <td>0.200</td> <td><u>MP5090</u></td> </tr> </tbody> </table> Attachments <input checked="" type="checkbox"/> Form 41 <input checked="" type="checkbox"/> Post-Stability Checks <input checked="" type="checkbox"/> Stability Checks <input type="checkbox"/> Flow Calibration <input checked="" type="checkbox"/> Calibration Certificate <input type="checkbox"/> Form 40 <input checked="" type="checkbox"/> Calibration Adjustment <input type="checkbox"/> Other _____ <input checked="" type="checkbox"/> Instrument Complies with Chapter 11D-8, FAC <input type="checkbox"/> Instrument Does Not Comply with Chapter 11D-8, FAC <input checked="" type="checkbox"/> Return to/Place into Evidentiary Use <input type="checkbox"/> Remain Out of Evidentiary Use <input checked="" type="checkbox"/> Conduct an Agency Inspection Before Evidentiary Use <table style="width:100%;"> <tr> <td style="width:50%; text-align: center;"> <u>Michael D. Haghighy</u> 2020.04.16 13:53:48 -04'00' </td> <td style="width:50%; text-align: center;"> <u>Brett Kirkland</u> 2020.04.17 08:52:04 -04'00' </td> </tr> <tr> <td style="text-align: center;">Tech Review / Date</td> <td style="text-align: center;">Admin Review / Date</td> </tr> </table>		Simulator	Serial Number	0.000	<u>MP5091</u>	Interferent	<u>MP5087</u>	0.050	<u>MP5088</u>	0.080	<u>MP5089</u>	0.200	<u>MP5090</u>	<u>Michael D. Haghighy</u> 2020.04.16 13:53:48 -04'00'	<u>Brett Kirkland</u> 2020.04.17 08:52:04 -04'00'	Tech Review / Date	Admin Review / Date																																
Simulator	Serial Number																																																	
0.000	<u>MP5091</u>																																																	
Interferent	<u>MP5087</u>																																																	
0.050	<u>MP5088</u>																																																	
0.080	<u>MP5089</u>																																																	
0.200	<u>MP5090</u>																																																	
<u>Michael D. Haghighy</u> 2020.04.16 13:53:48 -04'00'	<u>Brett Kirkland</u> 2020.04.17 08:52:04 -04'00'																																																	
Tech Review / Date	Admin Review / Date																																																	



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
2729 Fort Knox Blvd.
Bldg. 2, Suite 1300
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-006931, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-006931</u>	UNCERTAINTY* ±	
Owning Agency:	<u>FT WALTON BEACH PD</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>04/09/2020</u>	0.080 g/ 210 L	0.005
Calibration Time:	<u>09:30</u>	0.200 g/ 210 L	0.007
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration. *Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence (k=3).

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Thermometer temperatures are checked with NIST traceable Eutechnics 4400 digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the uses of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards.

This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

04/09/2020

Date

Shayla Platt

SHAYLA D PLATT,
Department Inspector

FDLE/ATP Form 69 January 2020

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: FT WALTON BEACH PD
Time of Inspection: 09:30

Date of Inspection: 04/09/2020

Serial Number: 80-006931
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201905A Exp: 05/14/2021	0.08g/210L Test (g/210L) Lot#:201905B Exp: 05/14/2021	0.20g/210L Test (g/210L) Lot#:201904D Exp: 04/30/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG931603 Exp: 11/12/2021
0.000	0.050	0.080	0.201	0.079
0.000	0.050	0.080	0.201	0.079
0.000	0.050	0.080	0.202	0.079
0.000	0.050	0.081	0.201	0.079
0.000	0.050	0.080	0.201	0.079
0.000	0.050	0.080	0.201	0.079
0.000	0.051	0.081	0.201	0.079
0.000	0.051	0.080	0.201	0.079
0.000	0.050	0.080	0.201	0.079
0.000	0.051	0.080	0.200	0.079
Standard Deviations	0.0004	0.0004	0.0004	0.0000

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5

Remarks:

M4

BK

2020.04.17
08:53:29
-04'00'

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Shayla Platt
SHAYLA D PLATT

Signature and Printed Name

04/09/2020
Date

Stability Checks

FT WALTON BEACH PD
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006931
 04/07/2020
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	06:34
Control Test	0.048	06:35
Air Blank	0.000	06:35
Control Test	0.048	06:36
Air Blank	0.000	06:37
Control Test	0.048	06:37
Air Blank	0.000	06:38
Control Test Stats		
Average	0.0480	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

FT WALTON BEACH PD
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006931
 04/07/2020
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	06:42
Control Test	0.078	06:43
Air Blank	0.000	06:44
Control Test	0.077	06:44
Air Blank	0.000	06:45
Control Test	0.078	06:46
Air Blank	0.000	06:46
Control Test Stats		
Average	0.0777	
Std Dev	0.0006	
Rel Std Dev(%)	0.7434	

FT WALTON BEACH PD
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006931
 04/07/2020
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	06:48
Control Test	0.199	06:48
Air Blank	0.000	06:49
Control Test	0.197	06:50
Air Blank	0.000	06:50
Control Test	0.197	06:51
Air Blank	0.000	06:52
Control Test Stats		
Average	0.1977	
Std Dev	0.0012	
Rel Std Dev(%)	0.5842	

wet



Operator's Signature



Operator's Signature



Operator's Signature

FT WALTON BEACH PD
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006931
 04/07/2020
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	06:57
Control Test	0.077	06:58
Air Blank	0.000	06:58
Control Test	0.077	06:58
Air Blank	0.000	06:59
Control Test	0.077	06:59
Air Blank	0.000	07:00
Control Test Stats		
Average	0.0770	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

Dry

MH



Operator's Signature

BK

2020.04.17
08:54:13 -04'00'

MA

BK

2020.04.17
08:55:01 -04'00'

FT WALTON BENCH PD
Intoxilyzer - Alcohol Analyzer
Model 8000
04/08/2020
SN 80-005931
07:20:54
Auto Calibration
Max Power Res UAlue = 73
Auto Range Res UAlue = 49

***** AUTO CAL DATA *****
 <<<<< CHANNEL 2 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 1.4670 (-0.0080)
 Sample #2 = 1.4740 (0.0210)
 Sample #3 = 1.4690 (0.0330)
 Sample #4 = 1.4570 (0.0450)
 Avg % Abs = 1.4667 (0.0330)
 STD DEV = 0.0087 (0.0120)
 REL STD DEV = 0.596 (36.364)

 Sol Value = 0.100 g/210L ***
 Fit value = 0.4762 mg/l %%%
 Samples Taken = 4, Discarded = 1
 Sum Io = 12356, Sum Io = 13164

 <<<<< CHANNEL 1 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 1.8010 (-0.0220)
 Sample #2 = 1.8180 (-0.0070)
 Sample #3 = 1.8050 (0.0240)
 Sample #4 = 1.7760 (0.0430)
 Avg % Abs = 1.7997 (0.0200)
 STD DEV = 0.0215 (0.0252)
 REL STD DEV = 1.195 (126.194)

 <<<<< CHANNEL 2 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 3.4020 (-0.0100)
 Sample #2 = 3.3730 (0.0340)
 Sample #3 = 3.3640 (0.0460)
 Sample #4 = 3.3590 (0.0510)
 Avg % Abs = 3.3653 (0.0437)
 STD DEV = 0.0071 (0.0087)
 REL STD DEV = 0.211 (20.008)

 Sol Value = 0.040 g/210L ***
 Fit value = 0.1905 mg/l %%%
 Samples Taken = 4, Discarded = 1
 Sum Io = 12382, Sum Io = 13174

 <<<<< CHANNEL 1 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 0.7390 (0.0040)
 Sample #2 = 0.7620 (0.0290)
 Sample #3 = 0.7350 (0.0480)
 Sample #4 = 0.7460 (0.0610)
 Avg % Abs = 0.7477 (0.0460)
 STD DEV = 0.0136 (0.0161)
 REL STD DEV = 1.816 (34.986)

 <<<<< CHANNEL 2 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 6.5720 (-0.0120)
 Sample #2 = 6.4800 (0.0830)
 Sample #3 = 6.4870 (0.0830)
 Sample #4 = 6.4810 (0.0970)
 Avg % Abs = 6.4827 (0.0877)
 STD DEV = 0.0038 (0.0081)
 REL STD DEV = 0.058 (9.220)

 Sol Value = 0.300 g/210L ***
 Fit value = 1.4286 mg/l %%%
 Samples Taken = 4, Discarded = 1
 Sum Io = 12347, Sum Io = 13152

 <<<<< CHANNEL 1 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 5.2250 (-0.0130)
 Sample #2 = 5.1410 (0.0740)
 Sample #3 = 5.1360 (0.0960)
 Sample #4 = 5.1510 (0.0970)
 Avg % Abs = 5.1427 (0.0891)
 STD DEV = 0.0076 (0.0130)
 REL STD DEV = 0.149 (14.607)

 <<<<< CHANNEL 2 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 9.4650 (-0.0120)
 Sample #2 = 9.3070 (0.1410)
 Sample #3 = 9.3130 (0.1380)
 Sample #4 = 9.3290 (0.1290)
 Avg % Abs = 9.3163 (0.1360)
 STD DEV = 0.0114 (0.0162)
 REL STD DEV = 0.122 (4.532)

 Sol Value = 0.200 g/210L ***
 Fit value = 0.9524 mg/l %%%
 Samples Taken = 4, Discarded = 1
 Sum Io = 12357, Sum Io = 13158

 <<<<< CHANNEL 1 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 3.5940 (-0.0140)
 Sample #2 = 3.5130 (0.0630)
 Sample #3 = 3.5220 (0.0710)
 Sample #4 = 3.5290 (0.0800)
 Avg % Abs = 3.5213 (0.0713)
 STD DEV = 0.0080 (0.0085)
 REL STD DEV = 0.228 (11.923)

 <<<<< CHANNEL 2 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 6.5720 (-0.0120)
 Sample #2 = 6.4800 (0.0830)
 Sample #3 = 6.4870 (0.0830)
 Sample #4 = 6.4810 (0.0970)
 Avg % Abs = 6.4827 (0.0877)
 STD DEV = 0.0038 (0.0081)
 REL STD DEV = 0.058 (9.220)

 Sol Value = 0.100 g/210L ***
 Fit value = 0.4762 mg/l %%%
 Samples Taken = 4, Discarded = 1
 Sum Io = 12356, Sum Io = 13164

 <<<<< CHANNEL 1 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 1.8010 (-0.0220)
 Sample #2 = 1.8180 (-0.0070)
 Sample #3 = 1.8050 (0.0240)
 Sample #4 = 1.7760 (0.0430)
 Avg % Abs = 1.7997 (0.0200)
 STD DEV = 0.0215 (0.0252)
 REL STD DEV = 1.195 (126.194)

 <<<<< CHANNEL 2 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 3.4020 (-0.0100)
 Sample #2 = 3.3730 (0.0340)
 Sample #3 = 3.3640 (0.0460)
 Sample #4 = 3.3590 (0.0510)
 Avg % Abs = 3.3653 (0.0437)
 STD DEV = 0.0071 (0.0087)
 REL STD DEV = 0.211 (20.008)

 Sol Value = 0.040 g/210L ***
 Fit value = 0.1905 mg/l %%%
 Samples Taken = 4, Discarded = 1
 Sum Io = 12382, Sum Io = 13174

 <<<<< CHANNEL 1 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 0.7390 (0.0040)
 Sample #2 = 0.7620 (0.0290)
 Sample #3 = 0.7350 (0.0480)
 Sample #4 = 0.7460 (0.0610)
 Avg % Abs = 0.7477 (0.0460)
 STD DEV = 0.0136 (0.0161)
 REL STD DEV = 1.816 (34.986)

 <<<<< CHANNEL 2 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 6.5720 (-0.0120)
 Sample #2 = 6.4800 (0.0830)
 Sample #3 = 6.4870 (0.0830)
 Sample #4 = 6.4810 (0.0970)
 Avg % Abs = 6.4827 (0.0877)
 STD DEV = 0.0038 (0.0081)
 REL STD DEV = 0.058 (9.220)

 Sol Value = 0.300 g/210L ***
 Fit value = 1.4286 mg/l %%%
 Samples Taken = 4, Discarded = 1
 Sum Io = 12347, Sum Io = 13152

 <<<<< CHANNEL 1 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 5.2250 (-0.0130)
 Sample #2 = 5.1410 (0.0740)
 Sample #3 = 5.1360 (0.0960)
 Sample #4 = 5.1510 (0.0970)
 Avg % Abs = 5.1427 (0.0891)
 STD DEV = 0.0076 (0.0130)
 REL STD DEV = 0.149 (14.607)

 <<<<< CHANNEL 2 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 9.4650 (-0.0120)
 Sample #2 = 9.3070 (0.1410)
 Sample #3 = 9.3130 (0.1380)
 Sample #4 = 9.3290 (0.1290)
 Avg % Abs = 9.3163 (0.1360)
 STD DEV = 0.0114 (0.0162)
 REL STD DEV = 0.122 (4.532)

 Sol Value = 0.200 g/210L ***
 Fit value = 0.9524 mg/l %%%
 Samples Taken = 4, Discarded = 1
 Sum Io = 12357, Sum Io = 13158

 <<<<< CHANNEL 1 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 3.5940 (-0.0140)
 Sample #2 = 3.5130 (0.0630)
 Sample #3 = 3.5220 (0.0710)
 Sample #4 = 3.5290 (0.0800)
 Avg % Abs = 3.5213 (0.0713)
 STD DEV = 0.0080 (0.0085)
 REL STD DEV = 0.228 (11.923)

 <<<<< CHANNEL 2 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 6.5720 (-0.0120)
 Sample #2 = 6.4800 (0.0830)
 Sample #3 = 6.4870 (0.0830)
 Sample #4 = 6.4810 (0.0970)
 Avg % Abs = 6.4827 (0.0877)
 STD DEV = 0.0038 (0.0081)
 REL STD DEV = 0.058 (9.220)

 Sol Value = 0.300 g/210L ***
 Fit value = 1.4286 mg/l %%%
 Samples Taken = 4, Discarded = 1
 Sum Io = 12347, Sum Io = 13152

 <<<<< CHANNEL 1 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 5.2250 (-0.0130)
 Sample #2 = 5.1410 (0.0740)
 Sample #3 = 5.1360 (0.0960)
 Sample #4 = 5.1510 (0.0970)
 Avg % Abs = 5.1427 (0.0891)
 STD DEV = 0.0076 (0.0130)
 REL STD DEV = 0.149 (14.607)

 <<<<< CHANNEL 2 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 9.4650 (-0.0120)
 Sample #2 = 9.3070 (0.1410)
 Sample #3 = 9.3130 (0.1380)
 Sample #4 = 9.3290 (0.1290)
 Avg % Abs = 9.3163 (0.1360)
 STD DEV = 0.0114 (0.0162)
 REL STD DEV = 0.122 (4.532)

 Sol Value = 0.200 g/210L ***
 Fit value = 0.9524 mg/l %%%
 Samples Taken = 4, Discarded = 1
 Sum Io = 12357, Sum Io = 13158

 <<<<< CHANNEL 1 >>>>>
 Sample % Abs (% Abs Ref)
 Sample #1 = 3.5940 (-0.0140)
 Sample #2 = 3.5130 (0.0630)
 Sample #3 = 3.5220 (0.0710)
 Sample #4 = 3.5290 (0.0800)
 Avg % Abs = 3.5213 (0.0713)
 STD DEV = 0.0080 (0.0085)
 REL STD DEV = 0.228 (11.923)

CAL ADJUSTMENT
#80-000931 SP

 Dry Gas H2O Adjust Results *****
 Barometric Pressure = 1013
 3 um H2O Adjust (mg/*10,000) = 417
 9 um H2O Adjust (mg/*10,000) = 464

 REL STD DEV = 0.846

***** CHANNEL 2 *****
 Sample #1 = 3328.00
 Sample #2 = 3350.00
 Sample #3 = 3315.00
 Sample #4 = 3371.00
 Average Result = 3345.3333
 STD DEV = 28.2902
 REL STD DEV = 0.846

***** CHANNEL 1 *****
 Sample #1 = 3413.00
 Sample #2 = 3398.00
 Sample #3 = 3325.00
 Sample #4 = 3454.00
 Average Result = 3392.3333
 STD DEV = 64.6664
 REL STD DEV = 1.907

***** CHANNEL 2 *****
 Sample #1 = 3328.00
 Sample #2 = 3350.00
 Sample #3 = 3315.00
 Sample #4 = 3371.00
 Average Result = 3345.3333
 STD DEV = 28.2902
 REL STD DEV = 0.846

***** CHANNEL 1 *****
 Sample #1 = 3413.00
 Sample #2 = 3398.00
 Sample #3 = 3325.00
 Sample #4 = 3454.00
 Average Result = 3392.3333
 STD DEV = 64.6664
 REL STD DEV = 1.907

80-006931

Checks

Post Cal Adjust Stability

FT WALTON BEACH PD
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006931
 04/09/2020
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	07:21
Control Test	0.051	07:22
Air Blank	0.000	07:22
Control Test	0.049	07:23
Air Blank	0.000	07:24
Control Test	0.050	07:24
Air Blank	0.000	07:25
Control Test Stats		
Average	0.0500	
Std Dev	0.0010	
Rel Std Dev(%)	2.0000	

SP

Operator's Signature

FT WALTON BEACH PD
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006931
 04/09/2020
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	07:08
Control Test	0.080	07:09
Air Blank	0.000	07:10
Control Test	0.080	07:10
Air Blank	0.000	07:11
Control Test	0.080	07:12
Air Blank	0.000	07:12
Control Test Stats		
Average	0.0800	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

SP

Operator's Signature

FT WALTON BEACH PD
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006931
 04/09/2020
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	07:02
Control Test	0.203	07:03
Air Blank	0.000	07:04
Control Test	0.202	07:04
Air Blank	0.000	07:05
Control Test	0.201	07:06
Air Blank	0.000	07:06
Control Test Stats		
Average	0.2020	
Std Dev	0.0010	
Rel Std Dev(%)	0.4950	

SP

Operator's Signature

FT WALTON BEACH PD
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006931
 04/09/2020
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	07:15
Control Test	0.081	07:15
Air Blank	0.000	07:16
Control Test	0.081	07:16
Air Blank	0.000	07:17
Control Test	0.080	07:17
Air Blank	0.000	07:18
Control Test Stats		
Average	0.0807	
Std Dev	0.0006	
Rel Std Dev(%)	0.7157	

DGB

SP

Operator's Signature

BK

Return Material Authorization

Ship to: CMI, Inc.
 Enforcement Electronics

Shipment to repair facility authorized by: James Martin on 9/3/2019

Items Returned: Instrument Supplies Other Describe: _____
Instrument Model: 8000 Serial Number: 80-006931

Bill To Address:
James Martin
Fort Walton Beach Police Department
7 Hollywood Boulevard NE
Fort Walton Beach, FL 32548-4920

Ship to Address:
FDLE Off-Site Mail Facility
c/o Florida Department of Law Enforcemen
Alcohol Testing Program
813B Lake Bradford Road
Tallahassee FL 32304

Reason for Return:

Internal printer, after a few minutes, prints constant stream of question marks. Turning
instrument off and then back on does not clear the problem. Owner believes that this will
be a warranty repair

Please choose one of the following options:

- 1. I _____, authorize all repairs.
- 2. I _____, authorize repairs up to \$ _____.
- 3. I require an estimate **BEFORE** any repairs will be authorized and/ or conducted.

Please contact: Name: James Martin

Phone #: 850-833-9683 Email: jmartin@fwb.org

ATP Contact Name: Patrick Murphy ATP Email: patrickmurphy@fdle.state.fl.us

MH
BK 2020.04.17
08:56:25
-04'00'



INSTRUMENT PROCESSING SHEET

Agency Fort Walton Beach PDS/N 80-006931Florida Department of
Law EnforcementDate In 8/16/2019 DI Completion Date _____ Ship P/U H/D CMI EE

Intake Performed By <u>DP</u> <input checked="" type="checkbox"/> Annual <input type="checkbox"/> Registration <input type="checkbox"/> Return from CMI / EE Visual Inspection: <input checked="" type="checkbox"/> Case <input checked="" type="checkbox"/> Handle <input checked="" type="checkbox"/> Keyboard <input type="checkbox"/> Dry Gas Shelf <input checked="" type="checkbox"/> Feet <input checked="" type="checkbox"/> Breath Tube <input checked="" type="checkbox"/> Ports <input checked="" type="checkbox"/> Screws Tight Other Equipment/ Accessories: <input checked="" type="checkbox"/> Power cord <input type="checkbox"/> Printer Cable <input type="checkbox"/> Static Bag <input type="checkbox"/> 12V DC Cable Notes: <u>Dry Gas Cuff missing</u> <u>Extra regulator enclosed.</u>	Quality Checks Performed By _____ <input checked="" type="checkbox"/> Breath Tube Screen <input checked="" type="checkbox"/> Replace External O-Rings <input type="checkbox"/> Instrument Set Up Verified <input type="checkbox"/> R-Value _____ <input type="checkbox"/> Flow Verification (L/s) Flow Column # <u>ATP102</u> 32 mm <u>.144</u> (.139 - .169) 36 mm <u>.160</u> (.156 - .190) 53 mm <u>.234</u> (.228 - .278) 103 mm <u>.476</u> (.447 - .547) <input type="checkbox"/> Barometric Pressure Check Gauge ID # _____ <input type="checkbox"/> Stability Checks <table border="1" style="width:100%; border-collapse: collapse; margin-top: 5px;"> <thead> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #/Exp</th> </tr> </thead> <tbody> <tr><td>0.050</td><td></td><td></td></tr> <tr><td>0.080</td><td></td><td></td></tr> <tr><td>0.200</td><td></td><td></td></tr> <tr><td>0.080 DGS</td><td>N/A</td><td></td></tr> </tbody> </table>	Simulator	Serial #	Lot #/Exp	0.050			0.080			0.200			0.080 DGS	N/A		Flow Calibration Performed By _____ Flow Column # _____ <input type="checkbox"/> 5L/min - 17mm <input type="checkbox"/> 15L/min - 53mm <input type="checkbox"/> 30L/min - 103mm <input type="checkbox"/> R-Value _____ <input type="checkbox"/> Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547) Maintenance Performed By _____ <input type="checkbox"/> Battery Replacement <input type="checkbox"/> Dry Gas Regulator Replacement <input type="checkbox"/> Breath Tube Replacement <input type="checkbox"/> Other _____ Temperature Checks Performed By _____ <input type="checkbox"/> Lab Temp °C _____ External Digital Therm. ID#: _____ <input type="checkbox"/> 34°C +-2 Serial #: _____ <input type="checkbox"/> 34°C +-2 Serial #: _____ <input type="checkbox"/> 34°C +-2 Serial #: _____																																	
Simulator	Serial #	Lot #/Exp																																																
0.050																																																		
0.080																																																		
0.200																																																		
0.080 DGS	N/A																																																	
Final Release Date 	Calibration Adjustment Performed By _____ Barometric Pressure Gauge _____ ID # _____ <table border="1" style="width:100%; border-collapse: collapse; margin-bottom: 5px;"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> <th>Lot Number</th> <th>Expiration</th> </tr> </thead> <tbody> <tr><td>0.000</td><td></td><td>N/A</td><td>N/A</td></tr> <tr><td>0.040</td><td></td><td></td><td></td></tr> <tr><td>0.100</td><td></td><td></td><td></td></tr> <tr><td>0.200</td><td></td><td></td><td></td></tr> <tr><td>0.300</td><td></td><td></td><td></td></tr> <tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr> </tbody> </table> <input type="checkbox"/> Post Calibration Adjustment Stability Checks <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> <th>Lot Number</th> <th>Expiration</th> </tr> </thead> <tbody> <tr><td>0.050</td><td></td><td></td><td></td></tr> <tr><td>0.080</td><td></td><td></td><td></td></tr> <tr><td>0.200</td><td></td><td></td><td></td></tr> <tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr> </tbody> </table>		Simulator	Serial Number	Lot Number	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Simulator	Serial Number	Lot Number	Expiration	0.050				0.080				0.200				0.080 DGS	N/A		
Simulator	Serial Number	Lot Number	Expiration																																															
0.000		N/A	N/A																																															
0.040																																																		
0.100																																																		
0.200																																																		
0.300																																																		
0.080 DGS	N/A																																																	
Simulator	Serial Number	Lot Number	Expiration																																															
0.050																																																		
0.080																																																		
0.200																																																		
0.080 DGS	N/A																																																	
Notes/Suggested Service: _____ _____ _____ _____ _____ _____	Department Inspection Performed By _____ Barometric Pressure ID# _____ Gauge _____ Instrument _____ Mouth Alcohol Solution Lot # _____ Acetone Stock Solution Lot # _____ <table border="1" style="width:100%; border-collapse: collapse; margin-bottom: 5px;"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> </tr> </thead> <tbody> <tr><td>0.000</td><td></td></tr> <tr><td>Interferent</td><td></td></tr> <tr><td>0.050</td><td></td></tr> <tr><td>0.080</td><td></td></tr> <tr><td>0.200</td><td></td></tr> </tbody> </table> Attachments <input type="checkbox"/> Form 41 <input type="checkbox"/> Post-Stability Checks <input type="checkbox"/> Stability Checks <input type="checkbox"/> Flow Calibration <input type="checkbox"/> Calibration Certificate <input type="checkbox"/> Form 40 <input type="checkbox"/> Calibration Adjustment <input type="checkbox"/> Other _____		Simulator	Serial Number	0.000		Interferent		0.050		0.080		0.200																																					
Simulator	Serial Number																																																	
0.000																																																		
Interferent																																																		
0.050																																																		
0.080																																																		
0.200																																																		
<input type="checkbox"/> Instrument Complies with Chapter 11D-8, FAC <input type="checkbox"/> Instrument Does Not Comply with Chapter 11D-8, FAC <input type="checkbox"/> Return to/Place into Evidentiary Use <input type="checkbox"/> Remain Out of Evidentiary Use <input type="checkbox"/> Conduct an Agency Inspection Before Evidentiary Use		Tech Review / Date _____ Admin Review / Date _____																																																

MK
 2020.04.
 17
 BK 08:57:04
 -04'00'

INTOXILYZER 80-006931

Dr. Pat Murphy

Our Intoxilyzer 8000 has the following errors/problems:

There is a loud hum coming from within the instrument itself. To me, the sound is synonymous with the bearings of a cooling fan going out on a desktop computer. When the instrument is started and the initial diagnostics are run it displays a voltage error and backs out to the "Ready Mode" screen.

Additionally, the Keyboard works fine during normal use, but when trying to access the Agency Inspection menus, suddenly the only thing I can do is change the date and time. I can press "I" for agency inspection, or "D" for diagnostic pressing the "return" button does nothing, and I cannot get the instrument to enter any menu other than time/date or control testing, but I cannot access any of the sub-menus "wet test, dry test." etc. etc.

I am unable to complete an inspection on the instrument or transmit any data, even if I could complete an inspection.

The gas cylinder valve on the instrument is from our previous 8000, the one inside the box but not installed is the original that came with this Intoxilyzer 8000 with the October 2017 purchase. I'm only including it should the instrument be required to return to CMI for warrantee work.

We have a new Quartermaster that handles our equipment

Mrs. Heather Murphy

Public Safety Quartermaster
Fort Walton Beach Police
850-833-9535 - Office
850-865-3895 - Cell

v/r

Sgt. James Martin #2042

Agency Inspector

MH

BK 2020.04.1
7 08:57:41
-04'00'

James Martin

From: Murphy, Patrick <PatrickMurphy@fdle.state.fl.us>
Sent: Thursday, August 8, 2019 9:32 AM
To: James Martin
Subject: RE: Intoxilyzer

Have we seen the instrument? If you haven't sent it yet, you should send it to us with a note about what you think is wrong and we'll check it out and then send it to CMI for you.

Patrick Murphy, Ph.D.

Department Inspector, Alcohol Testing Program
Florida Department of Law Enforcement
2331 Phillips Rd.
Tallahassee, FL 32308
(850) 617-1280 (work)
(850) 274-1338 (cell)
(850) 921-3787 (fax)

PLEASE NOTE : Florida has a very broad public records law. Most written communications to or from state officials regarding state business are considered to be public records and will be made available to the public and the media upon request. Your e-mail messages may, therefore, be subject to public disclosure.

From: James Martin [mailto:jmartin@fwb.org]
Sent: Thursday, August 08, 2019 10:01 AM
To: Murphy, Patrick
Subject: Intoxilyzer

Good Morning Dr. Murphy

How do I go about requesting a loaner Intoxilyzer 8000; ours is going to CMI for warrantee repair.

v/r

Sgt. James Martin #2042
Patrol Supervisor
B-Platoon, Delta Squad

M.S. Criminal Justice, University of Cincinnati

"Those who teach, learn."

My

BK 2020.04.17
08:59:13 -04'00'

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FT WALTON BEACH PD
Time of Inspection: 11:21

Date of Inspection: 08/28/2019

Serial Number: 80-006931
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08g/210L Test (g/210L) Lot#: _____ Exp: _____	0.20g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: _____ Exp: _____

Number of Simulators Used: _____

Remarks:
SKIPPED AI TO OPERATE INSTRUMENT

MH
BK 2020.04.17
08:59:46
-04'00"

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

PATRICK J MURPHY

Signature and Printed Name

08/28/2019
Date