

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 12:18

Date of Inspection: 02/27/2021

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:202005A Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:00521080A2 Exp: 02/05/2023
0.000	0.049	0.078	0.199	0.081
0.000	0.049	0.080	0.199	0.081
0.000	0.049	0.080	0.200	0.081

Number of Simulators Used: 5

Remarks:
CLEANED AREA

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

STEVE GASSEN

Signature and Printed Name

02/27/2021
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT -- INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 10:43

Date of Inspection: 01/28/2021

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:202005A Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:32518080A2 Exp: 02/05/2021
0.000	0.048	0.078	0.199	0.076
0.000	0.048	0.079	0.201	0.076
0.000	0.049	0.079	0.201	0.077


Number of Simulators Used: 5

Remarks:

CLEANED AREA

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

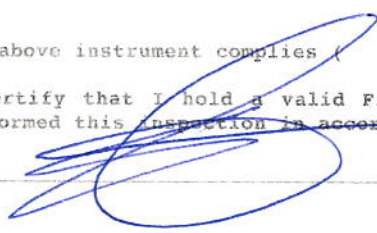

STEVE GASSEN

Signature and Printed Name

01/28/2021
Date