

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD
Time of Inspection: 12:21

Date of Inspection: 11/22/2021

Serial Number: 80-006926
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted	Yes	
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202005A Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34520080A1 Exp: 02/05/2023
0.000	0.047 / 0.047	0.078	0.190	0.077
0.000	0.048 / 0.048	0.078	0.192	0.077
0.000	0.058 / 0.048	0.078	0.194	0.076

Number of Simulators Used: 5


Remarks:

Time-Date changed. 05: Control Outside Tolerance.

checked connections. Ran test again. In compliance
DK

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DAVID KELLER

Signature and Printed Name

11/22/2021
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD
Time of Inspection: 15:49

Date of Inspection: 07/06/2021

Serial Number: 80-006926
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:202007A Exp: 07/21/2022	0.20g/210L Test (g/210L) Lot#:202005A Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34520080A1 Exp: 02/05/2023
0.000	0.048	0.077	0.193	0.082
0.000	0.048	0.078	0.195	0.082
0.000	0.048	0.078	0.196	0.082


Number of Simulators Used: 5

Remarks:

AI was completed after 20 simulator issues. All values within acceptable ranges. de

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DAVID KELLER

Signature and Printed Name

07/06/2021
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD
Time of Inspection: 14:42

Date of Inspection: 07/06/2021

Serial Number: 80-006926
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:202007A Exp: 07/21/2022	0.20g/210L Test (g/210L) Lot#:202005A Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:_____ Exp:_____
0.000	0.047	0.077	0.073 / 0.185	
0.000	0.048	0.077	0.073 / 0.187	
0.000	0.048	0.077	0.073 / 0.190	

Number of Simulators Used: 5


Remarks:

20: Control Outside Tolerance, Control Outside Tolerance. Non-compliance:OUTSIDE ACCEPTABLE RANGE OF .190 TO .210.

simulator lost power causing solution temp. to drop. once simulator was at proper temp. 20 solution was still outside acceptable range. Reseated top of simulator and completed entire agency inspection again AK

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DAVID KELLER

Signature and Printed Name

07/06/2021
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD
Time of Inspection: 15:49

Date of Inspection: 07/06/2021

Serial Number: 80-006926
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:202007A Exp: 07/21/2022	0.20g/210L Test (g/210L) Lot#:202005A Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34520080A1 Exp: 02/05/2023
0.000	0.048	0.077	0.193	0.082
0.000	0.048	0.078	0.195	0.082
0.000	0.048	0.078	0.196	0.082


Number of Simulators Used: 5

Remarks:

AI was completed after 20 simulator issues. All values within acceptable ranges. de

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DAVID KELLER

Signature and Printed Name

07/06/2021
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD
Time of Inspection: 14:42

Date of Inspection: 07/06/2021

Serial Number: 80-006926
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:202007A Exp: 07/21/2022	0.20g/210L Test (g/210L) Lot#:202005A Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:_____ Exp:_____
0.000	0.047	0.077	0.073 / 0.185	
0.000	0.048	0.077	0.073 / 0.187	
0.000	0.048	0.077	0.073 / 0.190	

Number of Simulators Used: 5


Remarks:

20: Control Outside Tolerance, Control Outside Tolerance. Non-compliance:OUTSIDE ACCEPTABLE RANGE OF .190 TO .210.

simulator lost power causing solution temp. to drop. once simulator was at proper temp. 20 solution was still outside acceptable range. Reseated top of simulator and completed entire agency inspection again AK

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DAVID KELLER

Signature and Printed Name

07/06/2021
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD
Time of Inspection: 12:13

Date of Inspection: 05/24/2021

Serial Number: 80-006926
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:202007A Exp: 07/21/2022	0.20g/210L Test (g/210L) Lot#:202005A Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34520080A1 Exp: 02/05/2023
0.000	0.047	0.078	0.196	0.082
0.000	0.048	0.078	0.197	0.082
0.000	0.047	0.078	0.198	0.082

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

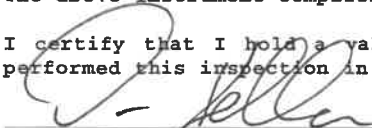

DAVID KELLER

Signature and Printed Name

05/24/2021
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD
Time of Inspection: 09:42

Date of Inspection: 05/24/2021

Serial Number: 80-006926
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted	Yes	
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08g/210L Test (g/210L) Lot#: _____ Exp: _____	0.20g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: _____ Exp: _____

Number of Simulators Used: 5


Remarks:

Time-Date changed. A F / M A:SEE NOTES. Non-compliance:SEE NOTES.

Mouth alcohol detected a BAC. Contacted Department Inspector who advised to redo AFE. No issues

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

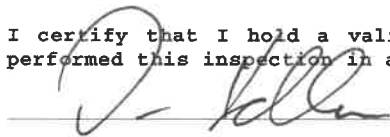

DAVID KELLER

Signature and Printed Name

05/24/2021
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD
Time of Inspection: 10:34

Date of Inspection: 04/20/2021

Serial Number: 80-006926
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:202005A Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34520080A1 Exp: 02/05/2023
0.000	0.000 / 0.047	0.080	0.195	0.082
0.000	0.000 / 0.048	0.080	0.195	0.082
0.000	0.000 / 0.049	0.080	0.197	0.081

Number of Simulators Used: 5

Remarks:

05: Control Outside Tolerance.

Tightened seal on simulator. Ran test again
DK

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DAVID KELLER

Signature and Printed Name

04/20/2021
Date