

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: Broward County SO

Serial Number: 80-007107

Time of Inspection:

Date of Inspection: May 2021

Software: 8100.27

CHECK OR TEST	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		
Alcohol Free Subject Test: 0.000		
Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect		
Diagnostic Check (Post-Inspection): OK		


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08g/210L Test (g/210L) Lot#: _____ Exp: _____	0.20g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: _____ Exp: _____

Number of Simulators Used: _____

Remarks: Inspection was not conducted as the instrument was sent to CMI, Inc for repairs.

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

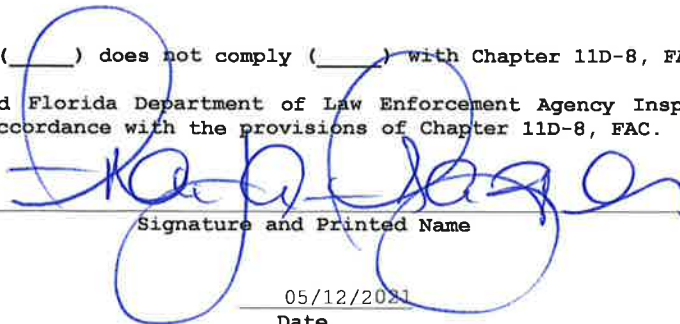

 Signature and Printed Name

 05/12/2021
 Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: Broward County SO
Time of Inspection:

Serial Number: 80-007107
Date of Inspection: July 2021

Software: 8100.27

CHECK OR TEST	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		
Alcohol Free Subject Test: 0.000		
Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect		
Diagnostic Check (Post-Inspection): OK		


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08g/210L Test (g/210L) Lot#: _____ Exp: _____	0.20g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: _____ Exp: _____

Number of Simulators Used: _____

Remarks: Inspection was not conducted as the instrument was sent to CMI, Inc for repairs.

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

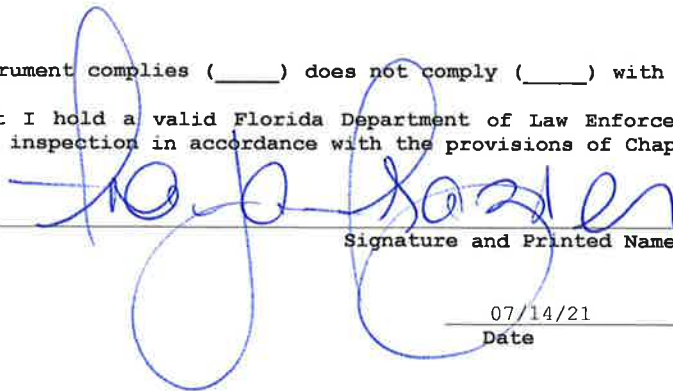

 Signature and Printed Name

07/14/21

 Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: Broward County SO
Time of Inspection:

Serial Number: 80-007107
Date of Inspection: November 2021

Software: 8100.27

CHECK OR TEST	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		
Alcohol Free Subject Test: 0.000		
Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect		
Diagnostic Check (Post-Inspection): OK		


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08g/210L Test (g/210L) Lot#: _____ Exp: _____	0.20g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: _____ Exp: _____

Number of Simulators Used: _____

Remarks: Inspection was not conducted as the instrument was sent to CMI, Inc for repairs.

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

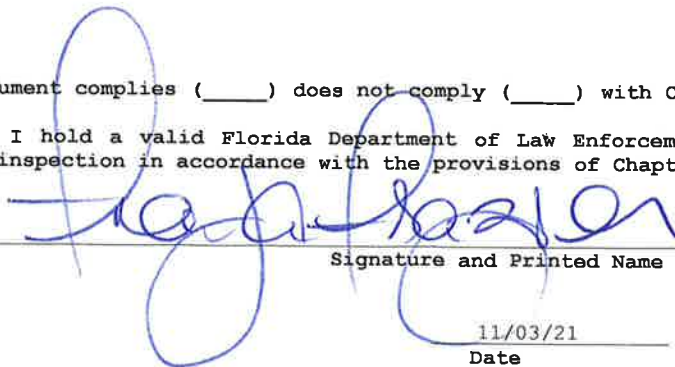

 Signature and Printed Name

 11/03/21
 Date