



INSTRUMENT PROCESSING SHEET

Agency Glades County SO

S/N 80-000947

Florida Department of Law Enforcement

Date In 7/6/2021 DI Completion Date \_\_\_\_\_

Ship  P/U  H/D  CMI  EE

<b>Intake</b> By MH _____ <input checked="" type="checkbox"/> Annual <input type="checkbox"/> Registration <input type="checkbox"/> Return from CMI / EE Visual Inspection: <input checked="" type="checkbox"/> Case <input checked="" type="checkbox"/> Handle <input checked="" type="checkbox"/> Keyboard <input checked="" type="checkbox"/> Dry Gas Shelf <input checked="" type="checkbox"/> Feet <input checked="" type="checkbox"/> Breath Tube <input checked="" type="checkbox"/> Ports <input checked="" type="checkbox"/> Screws Tight Other Equipment/ Accessories: <input type="checkbox"/> Power cord <input type="checkbox"/> Printer Cable <input checked="" type="checkbox"/> Static Bag <input type="checkbox"/> 12V DC Cable Notes: <u>DG Leak</u> _____ _____ _____ _____ _____ _____ _____ _____	<b>Quality Checks</b> By MH _____ Date <u>08/05/2021</u> <input checked="" type="checkbox"/> Breath Tube Screen <input checked="" type="checkbox"/> Replace External O-Rings <input checked="" type="checkbox"/> Instrument Set Up Verified <input checked="" type="checkbox"/> R-Value <u>235</u> <input checked="" type="checkbox"/> Flow Verification (L/s) Flow Column # <u>ATP 106</u> 32 mm <u>0.152</u> (.139 - .169) 36 mm <u>0.171</u> (.156 - .190) 53 mm <u>0.238</u> (.228 - .278) 103 mm <u>0.488</u> (.447 - .547) <input checked="" type="checkbox"/> Barometric Pressure Check Gauge ID # <u>28199</u> <input checked="" type="checkbox"/> Stability Checks <table border="1"> <thead> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #/Exp</th> </tr> </thead> <tbody> <tr> <td>0.050</td> <td>MP5092</td> <td>202010A 10/05/2022</td> </tr> <tr> <td>0.080</td> <td>MP5093</td> <td>202010B 10/05/2022</td> </tr> <tr> <td>0.200</td> <td>MP5097</td> <td>202010D 10/06/2022</td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td>AG026705 09/23/2022</td> </tr> </tbody> </table>	Simulator	Serial #	Lot #/Exp	0.050	MP5092	202010A 10/05/2022	0.080	MP5093	202010B 10/05/2022	0.200	MP5097	202010D 10/06/2022	0.080 DGS	N/A	AG026705 09/23/2022	<b>Flow Calibration</b> By _____ Date _____ Flow Column # _____ <input type="checkbox"/> 5L/min - 17mm <input type="checkbox"/> 15L/min - 53mm <input type="checkbox"/> 30L/min - 103mm <input type="checkbox"/> R-Value _____ <input type="checkbox"/> Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547) <b>Maintenance</b> By MH _____ <input type="checkbox"/> Battery Replacement <input checked="" type="checkbox"/> Dry Gas Regulator Replacement <input type="checkbox"/> Breath Tube Replacement <input checked="" type="checkbox"/> Other <u>DG Calibration</u> <b>DI Temp. Checks</b> By MH _____ <input checked="" type="checkbox"/> Lab Temp °C _____ External Digital Therm. ID#: <u>300504</u> <input checked="" type="checkbox"/> 34°C +/- .2 Serial #: <u>MP5092</u> <input checked="" type="checkbox"/> 34°C +/- .2 Serial #: <u>MP5093</u> <input checked="" type="checkbox"/> 34°C +/- .2 Serial #: <u>MP5097</u>
Simulator	Serial #	Lot #/Exp															
0.050	MP5092	202010A 10/05/2022															
0.080	MP5093	202010B 10/05/2022															
0.200	MP5097	202010D 10/06/2022															
0.080 DGS	N/A	AG026705 09/23/2022															

<b>Calibration Adjustment</b> By MH _____ Barometric Pressure Gauge <u>28663</u> ID # <u>1019</u> <table border="1"> <thead> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #</th> <th>Expiration</th> </tr> </thead> <tbody> <tr> <td>0.000</td> <td></td> <td>N/A</td> <td>N/A</td> </tr> <tr> <td>0.040</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.100</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.200</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.300</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td></td> <td></td> </tr> </tbody> </table> <input type="checkbox"/> Post Calibration Adjustment Stability Checks <table border="1"> <thead> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #</th> <th>Expiration</th> </tr> </thead> <tbody> <tr> <td>0.050</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.200</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td></td> <td></td> </tr> </tbody> </table> Notes/Suggested Service: <u>Unstable signal unable to calibration. Recommend repair.</u> <u>Sent to repair with leaking Regulator.</u> _____ _____ _____	Simulator	Serial #	Lot #	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Simulator	Serial #	Lot #	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			<b>Department Inspection</b> By MH _____ Barometric Pressure ID# <u>68639</u> Gauge _____ Instrument _____ Mouth Alcohol Solution Lot # <u>2021-A</u> Acetone Stock Solution Lot # <u>2020-A</u> <table border="1"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> </tr> </thead> <tbody> <tr> <td>0.000</td> <td>SD1014</td> </tr> <tr> <td>Interferent</td> <td>SD1015</td> </tr> <tr> <td>0.050</td> <td>MP4863</td> </tr> <tr> <td>0.080</td> <td>MP4864</td> </tr> <tr> <td>0.200</td> <td>MP5097</td> </tr> </tbody> </table> <b>Attachments</b> <input checked="" type="checkbox"/> Form 41 <input type="checkbox"/> Post-Stability Checks <input checked="" type="checkbox"/> Stability Checks <input type="checkbox"/> Flow Calibration <input checked="" type="checkbox"/> Calibration Certificate <input type="checkbox"/> Form 40 <input type="checkbox"/> Calibration Adjustment <input type="checkbox"/> Other _____ <input type="checkbox"/> Instrument Complies with Chapter 11D-8, FAC <input checked="" type="checkbox"/> Instrument Does Not Comply with Chapter 11D-8, FAC <input type="checkbox"/> Return to/Place into Evidentiary Use <input checked="" type="checkbox"/> Remain Out of Evidentiary Use <input type="checkbox"/> Conduct an Agency Inspection Before Evidentiary Use Tech Review / Date _____ Admin Review / Date _____	Simulator	Serial Number	0.000	SD1014	Interferent	SD1015	0.050	MP4863	0.080	MP4864	0.200	MP5097
Simulator	Serial #	Lot #	Expiration																																																										
0.000		N/A	N/A																																																										
0.040																																																													
0.100																																																													
0.200																																																													
0.300																																																													
0.080 DGS	N/A																																																												
Simulator	Serial #	Lot #	Expiration																																																										
0.050																																																													
0.080																																																													
0.200																																																													
0.080 DGS	N/A																																																												
Simulator	Serial Number																																																												
0.000	SD1014																																																												
Interferent	SD1015																																																												
0.050	MP4863																																																												
0.080	MP4864																																																												
0.200	MP5097																																																												

GLADES COUNTY S.O.  
 Intoxilyzer - Alcohol Analyzer  
 Model 8500  
 08/11/2021  
 S: 80-00947  
 09:03:35

Auto Calibration  
 Max Power Res Value = 85  
 Auto Range Res Value = 41

Sol Value = 0.000 g/210L \*\*\*  
 Fit value = 0.0000 mg/l %%%  
 Samples Taken = 4, Discarded = 1  
 Sum Io = 12727, Sum Lo = 12100

Channel 1 Data:  
 Sample % Abs (% Abs Ref)  
 Sample #1 = 0.2440 (-0.0200)  
 Sample #2 = 0.2120 (0.1590)  
 Sample #3 = -0.1630 (0.2920)  
 Sample #4 = 0.1530 (0.4280)  
 Avg % Abs = 0.1760 (0.2930)  
 STD DEV = 0.0316 (0.1345)  
 REL STD DEV = 17.941 (45.905)

Channel 2 Data:  
 Sample % Abs (% Abs Ref)  
 Sample #1 = 0.2210 (-0.0230)  
 Sample #2 = 0.1420 (0.1600)  
 Sample #3 = 0.1730 (0.2310)  
 Sample #4 = 0.1760 (0.2830)  
 Avg % Abs = 0.1637 (0.2247)  
 STD DEV = 0.0188 (0.0617)  
 REL STD DEV = 11.501 (27.483)

Sol Value = 0.040 g/210L \*\*\*  
 Fit value = 0.1905 mg/l %%%  
 Samples Taken = 4, Discarded = 1  
 Sum Io = 12652, Sum Lo = 12049

Channel 1 Data:  
 Sample % Abs (% Abs Ref)  
 Sample #1 = 0.9300 (-0.0250)  
 Sample #2 = 0.8640 (0.1080)  
 Sample #3 = 0.9240 (0.1580)  
 Sample #4 = 0.8690 (0.2290)  
 Avg % Abs = 0.8857 (0.1650)  
 STD DEV = 0.0333 (0.0668)  
 REL STD DEV = 3.759 (35.850)

Channel 2 Data:  
 Sample % Abs (% Abs Ref)  
 Sample #1 = 1.5770 (-0.0180)  
 Sample #2 = 1.5840 (0.0390)  
 Sample #3 = 1.5450 (0.1080)  
 Sample #4 = 1.4920 (0.1140)  
 Avg % Abs = 1.5403 (0.0870)  
 STD DEV = 0.1462 (0.0417)  
 REL STD DEV = 2.998 (47.905)

Sol Value = 0.100 g/210L \*\*\*  
 Fit value = 0.4762 mg/l %%%  
 Samples Taken = 4, Discarded = 1  
 Sum Io = 12596, Sum Lo = 12008

Channel 1 Data:  
 Sample % Abs (% Abs Ref)  
 Sample #1 = 1.8970 (-0.0190)  
 Sample #2 = 1.9930 (-0.0620)  
 Sample #3 = 1.9790 (0.0210)  
 Sample #4 = 1.9240 (0.1130)  
 Avg % Abs = 1.9653 (0.0240)  
 STD DEV = 0.0365 (0.0875)  
 REL STD DEV = 1.856 (364.744)

Channel 2 Data:  
 Sample % Abs (% Abs Ref)  
 Sample #1 = 3.4460 (-0.0070)  
 Sample #2 = 3.5350 (-0.0990)  
 Sample #3 = 3.5830 (-0.0720)  
 Sample #4 = 3.5430 (-0.0040)  
 Avg % Abs = 3.5537 (-0.0583)  
 STD DEV = 0.0257 (0.0490)  
 REL STD DEV = 0.724 (83.918)

Sol Value = 0.200 g/210L \*\*\*  
 Fit value = 0.9524 mg/l %%%  
 Samples Taken = 4, Discarded = 1  
 Sum Io = 12565, Sum Lo = 11993

Channel 1 Data:  
 Sample % Abs (% Abs Ref)  
 Sample #1 = 3.7570 (-0.0230)  
 Sample #2 = 3.7710 (0.0170)  
 Sample #3 = 3.7710 (0.0590)  
 Sample #4 = 3.7400 (0.1110)  
 Avg % Abs = 3.7607 (0.0623)  
 STD DEV = 0.0179 (0.0471)  
 REL STD DEV = 0.476 (75.543)

Channel 2 Data:  
 Sample % Abs (% Abs Ref)  
 Sample #1 = 6.8340 (-0.0340)  
 Sample #2 = 6.7860 (0.0150)  
 Sample #3 = 6.8030 (0.0220)  
 Sample #4 = 6.8090 (0.0800)  
 Avg % Abs = 6.8000 (0.0390)  
 STD DEV = 0.0108 (0.0357)  
 REL STD DEV = 0.159 (91.485)

Sol Value = 0.300 g/210L \*\*\*  
 Fit value = 1.4286 mg/l %%%  
 Samples Taken = 4, Discarded = 1  
 Sum Io = 12537, Sum Lo = 11969

Channel 1 Data:  
 Sample % Abs (% Abs Ref)  
 Sample #1 = 5.4790 (-0.0380)  
 Sample #2 = 5.4350 (0.0040)  
 Sample #3 = 5.4360 (0.0640)  
 Sample #4 = 5.4160 (0.0730)  
 Avg % Abs = 5.4290 (0.0470)  
 STD DEV = 0.0113 (0.0375)  
 REL STD DEV = 0.208 (79.809)

Channel 2 Data:  
 Sample % Abs (% Abs Ref)  
 Sample #1 = 9.8570 (-0.0240)  
 Sample #2 = 9.7850 (-0.0270)  
 Sample #3 = 9.8400 (-0.0040)  
 Sample #4 = 9.7950 (0.0270)  
 Avg % Abs = 9.8067 (-0.0013)  
 STD DEV = 0.0293 (0.0271)  
 REL STD DEV = 0.299 (2032.394)

\*\*\*\*\* AUTO CAL DATA \*\*\*\*\*

Channel 1 Data:  
 Sol Val = 0.000 mg/l or 0.000 g/210L  
 % Abs = 0.176  
 Std Dev = 0.03 Rel Std Dev = 17.94  
 Sol Val = 0.1905 mg/l or 0.040 g/210L  
 % Abs = 0.886  
 Std Dev = 0.03 Rel Std Dev = 3.76  
 Sol Val = 0.4762 mg/l or 0.100 g/210L  
 % Abs = 1.965  
 Std Dev = 0.04 Rel Std Dev = 1.86  
 Sol Val = 0.9524 mg/l or 0.200 g/210L  
 % Abs = 3.751  
 Std Dev = 0.02 Rel Std Dev = 0.48  
 Sol Val = 1.4286 mg/l or 0.300 g/210L  
 % Abs = 5.429  
 Std Dev = 0.01 Rel Std Dev = 0.21  
 Zero Order Coef = -414.95  
 First Order Coef = 2559.93  
 Second Order Coef = 26.44  
 Standard Deviation = 46.525543

Channel 2 Data:  
 Sol Val = 0.000 mg/l or 0.000 g/210L  
 % Abs = 0.164  
 Std Dev = 0.02 Rel Std Dev = 11.50  
 Sol Val = 0.1905 mg/l or 0.040 g/210L  
 % Abs = 1.540  
 Std Dev = 0.05 Rel Std Dev = 3.00  
 Sol Val = 0.4762 mg/l or 0.100 g/210L  
 % Abs = 3.554  
 Std Dev = 0.03 Rel Std Dev = 0.72  
 Sol Val = 0.9524 mg/l or 0.200 g/210L  
 % Abs = 6.800  
 Std Dev = 0.01 Rel Std Dev = 0.16  
 Sol Val = 1.4286 mg/l or 0.300 g/210L  
 % Abs = 9.807  
 Std Dev = 0.03 Rel Std Dev = 0.30  
 Zero Order Coef = -205.58  
 First Order Coef = 1342.47  
 Second Order Coef = 13.66  
 Standard Deviation = 22.471313

Solution Stats Quadratic Fit Chan 2

Act	Fit	Residual
g/210L	g/210L	g/210L
0.000	0.000	-0.0003
0.040	0.040	0.0002
0.100	0.099	0.0005
0.200	0.201	-0.0007
0.300	0.300	0.0003

Sol Value = 0.000 g/210L \*\*\*  
 Fit Value = 0.0000 mg/l %%%  
 Samples Taken = 4, Discarded = 1

Channel 1 Data:  
 Sample #1 = 2812.00  
 Sample #2 = 2843.00  
 Sample #3 = 2906.00  
 Sample #4 = 2928.00  
 Average Result = 2892.7333  
 STD DEV = 44.1177  
 REL STD DEV = 1.525

Channel 2 Data:  
 Sample #1 = 3312.00  
 Sample #2 = 3401.00  
 Sample #3 = 3357.00  
 Sample #4 = 3396.00  
 Average Result = 3394.6667  
 STD DEV = 24.0901  
 REL STD DEV = 0.712





\*\*\*\*\*  
 Dry Gas H2O Adjust Results \*\*\*\*\*  
 Barometric Pressure = 1019  
 3 um H2O Adjust (mg/l\*10,000) = 917  
 9 um H2O Adjust (mg/l\*10,000) = 425  
 \*\*\*\* AUTO CAL PASS

Solution Stats Quadratic Fit Chan 1

Act	Fit	Residual
g/210L	g/210L	g/210L
0.000	0.001	-0.0008
0.040	0.039	0.0007
0.100	0.099	0.0009
0.200	0.201	-0.0013
0.300	0.300	0.0005

**Optical Calibration**  
 SN: 80-000947  
 Agency: Glades County SO  
 Date: 8/11/21  
 By: MAA

TYPE OF TEST	SERIAL NUMBER	AGENCY	DATE	PERFORMED BY
Stabilities - POST	80-000947	Glades County SO	08/11/2021	MMO

0.05g/210L 0.047 to 0.053 <input type="checkbox"/>	0.08g/210L 0.077 to 0.083 <input type="checkbox"/>	0.20g/210L 0.194 to 0.206 <input type="checkbox"/>	DGS 0.08g/210L 0.077 to 0.083 <input type="checkbox"/>																																																																																																																																																
GLADES COUNTY S.O. Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-000947 08/11/2021 Software: 8100.27	GLADES COUNTY S.O. Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-000947 08/11/2021 Software: 8100.27	GLADES COUNTY S.O. Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-000947 08/11/2021 Software: 8100.27	GLADES COUNTY S.O. Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-000947 08/11/2021 Software: 8100.27																																																																																																																																																
<table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:49</td></tr> <tr><td>Control Test</td><td>0.051</td><td>09:50</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:50</td></tr> <tr><td>Control Test</td><td>0.049</td><td>09:51</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:51</td></tr> <tr><td>Control Test</td><td>0.050</td><td>09:52</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:53</td></tr> <tr><td colspan="3">Control Test Stats</td></tr> <tr><td>Average</td><td>0.0500</td><td></td></tr> <tr><td>Std Dev</td><td>0.0010</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>2.0000</td><td></td></tr> </tbody> </table>	Test	g/210L	Time	Air Blank	0.000	09:49	Control Test	0.051	09:50	Air Blank	0.000	09:50	Control Test	0.049	09:51	Air Blank	0.000	09:51	Control Test	0.050	09:52	Air Blank	0.000	09:53	Control Test Stats			Average	0.0500		Std Dev	0.0010		Rel Std Dev(%)	2.0000		<table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:53</td></tr> <tr><td>Control Test</td><td>0.084</td><td>09:54</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:55</td></tr> <tr><td>Control Test</td><td>0.079</td><td>09:55</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:56</td></tr> <tr><td>Control Test</td><td>0.080</td><td>09:57</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:57</td></tr> <tr><td colspan="3">Control Test Stats</td></tr> <tr><td>Average</td><td>0.0810</td><td></td></tr> <tr><td>Std Dev</td><td>0.0026</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>3.2664</td><td></td></tr> </tbody> </table>	Test	g/210L	Time	Air Blank	0.000	09:53	Control Test	0.084	09:54	Air Blank	0.000	09:55	Control Test	0.079	09:55	Air Blank	0.000	09:56	Control Test	0.080	09:57	Air Blank	0.000	09:57	Control Test Stats			Average	0.0810		Std Dev	0.0026		Rel Std Dev(%)	3.2664		<table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:58</td></tr> <tr><td>Control Test</td><td>0.199</td><td>09:59</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:59</td></tr> <tr><td>Control Test</td><td>0.198</td><td>10:00</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:00</td></tr> <tr><td>Control Test</td><td>0.198</td><td>10:01</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:02</td></tr> <tr><td colspan="3">Control Test Stats</td></tr> <tr><td>Average</td><td>0.1983</td><td></td></tr> <tr><td>Std Dev</td><td>0.0006</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>0.2911</td><td></td></tr> </tbody> </table>	Test	g/210L	Time	Air Blank	0.000	09:58	Control Test	0.199	09:59	Air Blank	0.000	09:59	Control Test	0.198	10:00	Air Blank	0.000	10:00	Control Test	0.198	10:01	Air Blank	0.000	10:02	Control Test Stats			Average	0.1983		Std Dev	0.0006		Rel Std Dev(%)	0.2911		<table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>10:04</td></tr> <tr><td>Control Test</td><td>0.077</td><td>10:04</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:05</td></tr> <tr><td>Control Test</td><td>0.079</td><td>10:05</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:06</td></tr> <tr><td>Control Test</td><td>0.077</td><td>10:06</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:06</td></tr> <tr><td colspan="3">Control Test Stats</td></tr> <tr><td>Average</td><td>0.0777</td><td></td></tr> <tr><td>Std Dev</td><td>0.0012</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>1.4867</td><td></td></tr> </tbody> </table>	Test	g/210L	Time	Air Blank	0.000	10:04	Control Test	0.077	10:04	Air Blank	0.000	10:05	Control Test	0.079	10:05	Air Blank	0.000	10:06	Control Test	0.077	10:06	Air Blank	0.000	10:06	Control Test Stats			Average	0.0777		Std Dev	0.0012		Rel Std Dev(%)	1.4867	
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	09:49																																																																																																																																																	
Control Test	0.051	09:50																																																																																																																																																	
Air Blank	0.000	09:50																																																																																																																																																	
Control Test	0.049	09:51																																																																																																																																																	
Air Blank	0.000	09:51																																																																																																																																																	
Control Test	0.050	09:52																																																																																																																																																	
Air Blank	0.000	09:53																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0500																																																																																																																																																		
Std Dev	0.0010																																																																																																																																																		
Rel Std Dev(%)	2.0000																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	09:53																																																																																																																																																	
Control Test	0.084	09:54																																																																																																																																																	
Air Blank	0.000	09:55																																																																																																																																																	
Control Test	0.079	09:55																																																																																																																																																	
Air Blank	0.000	09:56																																																																																																																																																	
Control Test	0.080	09:57																																																																																																																																																	
Air Blank	0.000	09:57																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0810																																																																																																																																																		
Std Dev	0.0026																																																																																																																																																		
Rel Std Dev(%)	3.2664																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	09:58																																																																																																																																																	
Control Test	0.199	09:59																																																																																																																																																	
Air Blank	0.000	09:59																																																																																																																																																	
Control Test	0.198	10:00																																																																																																																																																	
Air Blank	0.000	10:00																																																																																																																																																	
Control Test	0.198	10:01																																																																																																																																																	
Air Blank	0.000	10:02																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.1983																																																																																																																																																		
Std Dev	0.0006																																																																																																																																																		
Rel Std Dev(%)	0.2911																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	10:04																																																																																																																																																	
Control Test	0.077	10:04																																																																																																																																																	
Air Blank	0.000	10:05																																																																																																																																																	
Control Test	0.079	10:05																																																																																																																																																	
Air Blank	0.000	10:06																																																																																																																																																	
Control Test	0.077	10:06																																																																																																																																																	
Air Blank	0.000	10:06																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0777																																																																																																																																																		
Std Dev	0.0012																																																																																																																																																		
Rel Std Dev(%)	1.4867																																																																																																																																																		
Operator's Signature 	Operator's Signature 	Operator's Signature 	Operator's Signature 																																																																																																																																																

TYPE OF TEST	SERIAL NUMBER	AGENCY	DATE	PERFORMED BY
Stabilities <del>POST</del>	80-000947	Glades County SO	8/11/21	MMK

0.05g/210L 0.047 to 0.053 <input checked="" type="checkbox"/>	0.08g/210L 0.077 to 0.083 <input type="checkbox"/>	0.20g/210L 0.194 to 0.206 <input type="checkbox"/>	DGS 0.08g/210L 0.077 to 0.083 <input type="checkbox"/>																																				
<p>GLADES COUNTY S.O. Intoxilyzer - Alconoc Analyzer Model 8000 SN 80-000947 08/11/2021 Software: 8.00.07</p> <table border="1"> <thead> <tr> <th>Test</th> <th></th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:45</td></tr> <tr><td>Control Test</td><td>0.038</td><td>09:45</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:46</td></tr> <tr><td>Control Test</td><td>0.051</td><td>09:47</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:47</td></tr> <tr><td>Control Test</td><td>0.048</td><td>09:48</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:48</td></tr> <tr><td colspan="3">Control Test Stats</td></tr> <tr><td>Average</td><td>0.0457</td><td></td></tr> <tr><td>Std Dev</td><td>0.0068</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>14.9055</td><td></td></tr> </tbody> </table> <p>MMK</p> <p>Operator's Signature</p>	Test		Time	Air Blank	0.000	09:45	Control Test	0.038	09:45	Air Blank	0.000	09:46	Control Test	0.051	09:47	Air Blank	0.000	09:47	Control Test	0.048	09:48	Air Blank	0.000	09:48	Control Test Stats			Average	0.0457		Std Dev	0.0068		Rel Std Dev(%)	14.9055		<p>Tighten simulator Calibration port after 0.038g/210L May have been loose.</p>		
Test		Time																																					
Air Blank	0.000	09:45																																					
Control Test	0.038	09:45																																					
Air Blank	0.000	09:46																																					
Control Test	0.051	09:47																																					
Air Blank	0.000	09:47																																					
Control Test	0.048	09:48																																					
Air Blank	0.000	09:48																																					
Control Test Stats																																							
Average	0.0457																																						
Std Dev	0.0068																																						
Rel Std Dev(%)	14.9055																																						

TYPE OF TEST	SERIAL NUMBER	AGENCY	DATE	PERFORMED BY
Stabilities	80-000947	Glades County SO	08/05/21	MX

0.05g/210L 0.047 to 0.053 <input checked="" type="checkbox"/>	0.08g/210L 0.077 to 0.083 <input checked="" type="checkbox"/>	0.20g/210L 0.194 to 0.206 <input checked="" type="checkbox"/>	DGS 0.08g/210L 0.077 to 0.083 <input checked="" type="checkbox"/>																																																																																																																																																
<p>GLADES COUNTY S.O. Intoxilyzer - Alconol Analyzer Model 8000 SN 80-000947 08/05/2021 Software: 8100.27</p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:53</td></tr> <tr><td>Control Test</td><td>0.048</td><td>09:54</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:55</td></tr> <tr><td>Control Test</td><td>0.050</td><td>09:55</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:56</td></tr> <tr><td>Control Test</td><td>0.049</td><td>09:57</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:57</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0490</td><td></td></tr> <tr><td>Std Dev</td><td>0.0010</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>2.0408</td><td></td></tr> </tbody> </table> <p>Operator's Signature: <i>MX</i></p>	Test	g/210L	Time	Air Blank	0.000	09:53	Control Test	0.048	09:54	Air Blank	0.000	09:55	Control Test	0.050	09:55	Air Blank	0.000	09:56	Control Test	0.049	09:57	Air Blank	0.000	10:57	Control Test Stats			Average	0.0490		Std Dev	0.0010		Rel Std Dev(%)	2.0408		<p>GLADES COUNTY S.O. Intoxilyzer - Alconol Analyzer Model 8000 SN 80-000947 08/05/2021 Software: 8100.27</p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:59</td></tr> <tr><td>Control Test</td><td>0.078</td><td>09:59</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:00</td></tr> <tr><td>Control Test</td><td>0.078</td><td>10:01</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:01</td></tr> <tr><td>Control Test</td><td>0.077</td><td>10:02</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:02</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0777</td><td></td></tr> <tr><td>Std Dev</td><td>0.0006</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>0.7434</td><td></td></tr> </tbody> </table> <p>Operator's Signature: <i>MX</i></p>	Test	g/210L	Time	Air Blank	0.000	09:59	Control Test	0.078	09:59	Air Blank	0.000	10:00	Control Test	0.078	10:01	Air Blank	0.000	10:01	Control Test	0.077	10:02	Air Blank	0.000	10:02	Control Test Stats			Average	0.0777		Std Dev	0.0006		Rel Std Dev(%)	0.7434		<p>GLADES COUNTY S.O. Intoxilyzer - Alconol Analyzer Model 8000 SN 80-000947 08/05/2021 Software: 8100.27</p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>10:05</td></tr> <tr><td>Control Test</td><td>0.201</td><td>10:05</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:06</td></tr> <tr><td>Control Test</td><td>0.200</td><td>10:07</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:07</td></tr> <tr><td>Control Test</td><td>0.201</td><td>10:08</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:08</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.2007</td><td></td></tr> <tr><td>Std Dev</td><td>0.0006</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>0.2877</td><td></td></tr> </tbody> </table> <p>Operator's Signature: <i>MX</i></p>	Test	g/210L	Time	Air Blank	0.000	10:05	Control Test	0.201	10:05	Air Blank	0.000	10:06	Control Test	0.200	10:07	Air Blank	0.000	10:07	Control Test	0.201	10:08	Air Blank	0.000	10:08	Control Test Stats			Average	0.2007		Std Dev	0.0006		Rel Std Dev(%)	0.2877		<p>GLADES COUNTY S.O. Intoxilyzer - Alconol Analyzer Model 8000 SN 80-000947 08/05/2021 Software: 8100.27</p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>10:11</td></tr> <tr><td>Control Test</td><td>0.083</td><td>10:12</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:12</td></tr> <tr><td>Control Test</td><td>0.080</td><td>10:13</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:13</td></tr> <tr><td>Control Test</td><td>0.082</td><td>10:14</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:14</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0817</td><td></td></tr> <tr><td>Std Dev</td><td>0.0015</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>1.8704</td><td></td></tr> </tbody> </table> <p>Operator's Signature: <i>MX</i></p>	Test	g/210L	Time	Air Blank	0.000	10:11	Control Test	0.083	10:12	Air Blank	0.000	10:12	Control Test	0.080	10:13	Air Blank	0.000	10:13	Control Test	0.082	10:14	Air Blank	0.000	10:14	Control Test Stats			Average	0.0817		Std Dev	0.0015		Rel Std Dev(%)	1.8704	
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	09:53																																																																																																																																																	
Control Test	0.048	09:54																																																																																																																																																	
Air Blank	0.000	09:55																																																																																																																																																	
Control Test	0.050	09:55																																																																																																																																																	
Air Blank	0.000	09:56																																																																																																																																																	
Control Test	0.049	09:57																																																																																																																																																	
Air Blank	0.000	10:57																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0490																																																																																																																																																		
Std Dev	0.0010																																																																																																																																																		
Rel Std Dev(%)	2.0408																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	09:59																																																																																																																																																	
Control Test	0.078	09:59																																																																																																																																																	
Air Blank	0.000	10:00																																																																																																																																																	
Control Test	0.078	10:01																																																																																																																																																	
Air Blank	0.000	10:01																																																																																																																																																	
Control Test	0.077	10:02																																																																																																																																																	
Air Blank	0.000	10:02																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0777																																																																																																																																																		
Std Dev	0.0006																																																																																																																																																		
Rel Std Dev(%)	0.7434																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	10:05																																																																																																																																																	
Control Test	0.201	10:05																																																																																																																																																	
Air Blank	0.000	10:06																																																																																																																																																	
Control Test	0.200	10:07																																																																																																																																																	
Air Blank	0.000	10:07																																																																																																																																																	
Control Test	0.201	10:08																																																																																																																																																	
Air Blank	0.000	10:08																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.2007																																																																																																																																																		
Std Dev	0.0006																																																																																																																																																		
Rel Std Dev(%)	0.2877																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	10:11																																																																																																																																																	
Control Test	0.083	10:12																																																																																																																																																	
Air Blank	0.000	10:12																																																																																																																																																	
Control Test	0.080	10:13																																																																																																																																																	
Air Blank	0.000	10:13																																																																																																																																																	
Control Test	0.082	10:14																																																																																																																																																	
Air Blank	0.000	10:14																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0817																																																																																																																																																		
Std Dev	0.0015																																																																																																																																																		
Rel Std Dev(%)	1.8704																																																																																																																																																		

**Return Material Authorization**

**Ship to:**  CMI, Inc.  
 Enforcement Electronics

Shipment to repair facility authorized by: Sergeant J. Bonilla on 08/18/2021

**Items Returned:** Instrument  Supplies  Other  Describe: \_\_\_\_\_

Instrument Model: Intoxilyzer 8000 Serial Number: 80-000947

Bill To Address:  
Glades County SO  
1297 E. State Road 78  
Moore Haven, Fl., 33471

Ship to Address:  
FDLE ATP  
ATTN: Michael Haughey  
4700 Terminal Drive Suite 1  
Fort Myers FL 33907

**Reason for Return:**

Unable to calibrate instrument. Checked DVMS 3 is higher then 9, and when flicked signal jumps up. Dry Gas leaks.

**Please choose one of the following options:**

- 1. I \_\_\_\_\_, authorize all repairs.
- 2. I \_\_\_\_\_, authorize repairs up to \$\_\_\_\_\_.
- 3. I require an estimate **BEFORE** any repairs will be authorized and/ or conducted.

Please contact: Name: Sergeant J. Bonilla

Phone #: 863-946-1600 Email: jbonilla@gladessheriff.org

ATP Contact Name: Michael Haughey ATP Email: michaelhaughey@fdle.state.fl.us

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: GLADES COUNTY S.O.  
Time of Inspection: 09:02

Date of Inspection: 08/05/2021

Serial Number: 80-000947  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08g/210L Test (g/210L) Lot#: _____ Exp: _____	0.20g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: _____ Exp: _____

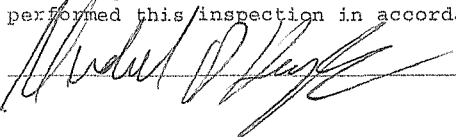
Number of Simulators Used: \_\_\_\_\_

Remarks:

COMPLAINCE NOT DETERMINED. BYPASS AI.

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MICHAEL D HAUGHEY

Signature and Printed Name

08/05/2021  
Date