

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 16:08

Date of Inspection: 08/10/2022

Serial Number: 80-000782

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402328118 Exp: 01/20/2025
0.000	0.049	0.078	0.198	0.083
0.000	0.049	0.079	0.199	0.083
0.000	0.049	0.079	0.199	0.082


Number of Simulators Used: 5

Remarks:

NA

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE

Signature and Printed Name

08/10/2022

Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 16:08

Date of Inspection: 08/10/2022

Serial Number: 80-000782

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402328118 Exp: 01/20/2025
0.000	0.049	0.078	0.198	0.083
0.000	0.049	0.079	0.199	0.083
0.000	0.049	0.079	0.199	0.082


Number of Simulators Used: 5

Remarks:

NA

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE

Signature and Printed Name

08/10/2022

Date

Florida Department of Law Enforcement

Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 21:53

Date of Inspection: 09/29/2022

Serial Number: 80-000782

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:2402328118 Exp: 01/20/2025
0.000	0.047	0.078	0.196	0.082
0.000	0.048	0.078	0.196	0.083
0.000	0.049	0.079	0.197	0.083

Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL

Signature and Printed Name

09/29/2022
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 13:49

Date of Inspection: 10/03/2022

Serial Number: 80-000782

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:2402328118 Exp: 01/20/2025
0.000	0.048	0.078	0.196	0.083
0.000	0.049	0.079	0.198	0.083
0.000	0.048	0.078	0.197	0.083

Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL

Signature and Printed Name

10/03/2022

Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 14:16

Date of Inspection: 11/15/2022

Serial Number: 80-000782

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:2402328118 Exp: 01/20/2025
0.000	0.048	0.078	0.198	0.083
0.000	0.048	0.079	0.198	0.083
0.000	0.048	0.079	0.199	0.082

Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL

Signature and Printed Name

11/15/2022
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 14:25

Date of Inspection: 12/03/2022

Serial Number: 80-000782

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:2402328118 Exp: 01/20/2025
0.000	0.048	0.078	0.195	0.083
0.000	0.048	0.078	0.195	0.083
0.000	0.048	0.078	0.195	0.082


Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

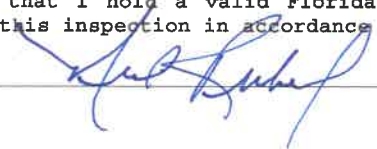

NEIL F RUBEL

Signature and Printed Name

12/03/2022

Date