

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: ORANGE COUNTY S.O.
Time of Inspection: 10:46

Date of Inspection: 10/26/2022

Serial Number: 80-000963
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted	Yes	No <i>OK</i>
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#: 202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#: 202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 07622080A3 Exp: 05/05/2024
0.000	0.048	0.079	0.199	0.077
0.000	0.049	0.078	0.200	0.077
0.000	0.049	0.079	0.200	0.077

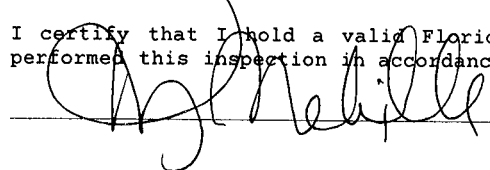
Number of Simulators Used: 5

Remarks:

Time and date adjusted during Agency Inspection. Notified
D.I. P. Nicodemo. *OK*

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 _____
Signature and Printed Name

KELLY M MELVILLE

10/26/2022
Date