

AMENDED

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: HOLMES BEACH PD
Time of Inspection: 14:53

Date of Inspection: 12/06/2022

Serial Number: 80-006692
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#: 202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#: 202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 402419647 Exp: 04/14/2025
0.000	0.049	0.079	0.198	0.079
0.000	0.048	0.079	0.198	0.079
0.000	0.049	0.078	0.198	0.079

Number of Simulators Used: 5

Remarks:

SOLUTION LOT #S WERE INCORRECT ON LAST INSPECTION ON 12/06/2022, at 13:23HRS
INSPECTION WAS REPEATED and correct lot #'s were entered AD

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Signature and Printed Name

ADAM B DESANTIS

12/06/2022
Date

AMENDED

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: HOLMES BEACH PD
Time of Inspection: 14:53

Date of Inspection: 12/06/2022

Serial Number: 80-006692
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#: 202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#: 202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 402419647 Exp: 04/14/2025
0.000	0.049	0.079	0.198	0.079
0.000	0.048	0.079	0.198	0.079
0.000	0.049	0.078	0.198	0.079


Number of Simulators Used: 5

Remarks:

SOLUTION LOT #S WERE INCORRECT ON LAST INSPECTION ON 12/06/2022, AT 13:23 HRS
INSPECTION WAS REPEATED AND CORRECT LOT #'S WERE ENTERED

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

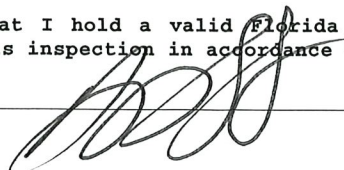

ADAM B DESANTIS
Signature and Printed Name

12/06/2022
Date