

Type of Test	Serial Number	Agency	Date	Performed By
Stabilities	80-000812	Hernando CSO	07/29/2022	TDG MB

0.05g/210L	0.08g/210L	0.20g/210L	DGS 0.08g/210L
0.047 to 0.053	0.077 to 0.083	0.194 to 0.206	0.077 to 0.083
HERNANDO COUNTY S.O. Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-000812 07/29/2022 Software: 8100.27 Test g/210L Time Air Blank 0.000 12:10 Control Test 0.051 12:11 Air Blank 0.000 12:11 Control Test 0.051 12:12 Air Blank 0.000 12:12 Control Test 0.052 12:13 Air Blank 0.000 12:14 Control Test Stats Average 0.0513 Std Dev 0.0006 Rel Std Dev(%) 1.1247	HERNANDO COUNTY S.O. Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-000812 07/29/2022 Software: 8100.27 Test g/210L Time Air Blank 0.000 12:16 Control Test 0.080 12:17 Air Blank 0.000 12:18 Control Test 0.080 12:18 Air Blank 0.000 12:19 Control Test 0.080 12:19 Air Blank 0.000 12:20 Control Test Stats Average 0.0800 Std Dev 0.0000 Rel Std Dev(%) 0.0000	HERNANDO COUNTY S.O. Intoxilyzer - Alcohol Analyzer Model 8000 SN 81-000812 07/29/2022 Software: 8100.27 Test g/210L Time Air Blank 0.000 12:27 Control Test 0.200 12:28 Air Blank 0.000 12:29 Control Test 0.201 12:29 Air Blank 0.000 12:30 Control Test 0.201 12:31 Air Blank 0.000 12:31 Control Test Stats Average 0.2007 Std Dev 0.0006 Rel Std Dev(%) 0.2877	HERNANDO COUNTY S.O. Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-000812 07/29/2022 Software: 8100.27 Test g/210L Time Air Blank 0.000 12:32 Control Test 0.081 12:33 Air Blank 0.000 12:33 Control Test 0.081 12:34 Air Blank 0.000 12:34 Control Test 0.080 12:34 Air Blank 0.000 12:35 Control Test Stats Average 0.0807 Std Dev 0.0006 Rel Std Dev(%) 0.7157
MB Operator's Signature	MB Operator's Signature	MB Operator's Signature	MB Operator's Signature

Comments:

Flow Calibration

80-000812

7/29/2022

ML

#1

HERNANDO COUNTY S.O.
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000812
07/29/2022
Software: 8100.27

Flow Rate Calibration*****

1: Rate (Liters/min) = 5
SQRT(Diff) = 7.141
2: Rate (Liters/min) = 15
SQRT(Diff) = 11.574
3: Rate (Liters/min) = 30
SQRT(Diff) = 21.000
Dependent Data Scale Factor = 100000 L/min
Independent Data Scale Factor = 256
Rounded Slope = 692
Rounded Intercept = -677269
Correlation = 0.99595

During the post-cal verification, the 53 mm flow rate was still outside nominal. Repeated the flow cal.

#2

HERNANDO COUNTY S.O.
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000812
07/29/2022
Software: 8100.27

Flow Rate Calibration*****

1: Rate (Liters/min) = 5
SQRT(Diff) = 6.781
2: Rate (Liters/min) = 15
SQRT(Diff) = 11.398
3: Rate (Liters/min) = 30
SQRT(Diff) = 20.879
Dependent Data Scale Factor = 100000 L/min
Independent Data Scale Factor = 256
Rounded Slope = 682
Rounded Intercept = -605124
Correlation = 0.99667

All post-cal values were within nominal.

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: HERNANDO COUNTY S.O.
Time of Inspection: 12:47

Date of Inspection: 08/01/2022

Serial Number: 80-000812
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202201C Exp: 01/11/2024	0.08g/210L Test (g/210L) Lot#:202201D Exp: 01/18/2024	0.20g/210L Test (g/210L) Lot#:202201E Exp: 01/18/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:00521080A2 Exp: 02/05/2023
0.000	0.050	0.080	0.200	0.082
0.000	0.051	0.080	0.200	0.082
0.000	0.050	0.080	0.200	0.081
0.000	0.051	0.080	0.201	0.082
0.000	0.051	0.081	0.200	0.081
0.000	0.050	0.080	0.200	0.082
0.000	0.050	0.080	0.200	0.082
0.000	0.051	0.080	0.200	0.082
0.000	0.050	0.081	0.201	0.081
0.000	0.050	0.080	0.200	0.081

Standard Deviations	0.0005	0.0004	0.0004	0.0005
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0004 Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



TAYLOR D GUTSCHOW

Signature and Printed Name

08/01/2022
Date



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
4700 Terminal Drive, Suite 1
Ft. Myers, FL 33907

This is to certify the calibration of Intoxilyzer 8000 serial number 80-000812, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-000812</u>	UNCERTAINTY* $\pm$
Owning Agency:	<u>HERNANDO COUNTY S.O.</u>	0.050 g/ 210 L 0.004
Calibration Date:	<u>08/01/2022</u>	0.080 g/ 210 L 0.004
Calibration Time:	<u>12:47</u>	0.200 g/ 210 L 0.007
		0.080 g/ 210 L Dry Gas Control 0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.

*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence (k=3).


The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards. This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

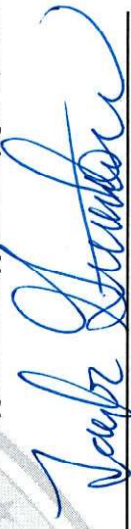

08/01/2022

Date
TAYLOR D GUTSCHOW,
Department Inspector

FDLE/ATP Form 69 December 2021
Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality