

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 15:12

Date of Inspection: 12/11/2023

Serial Number: 80-000759
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.049	0.078	0.195	0.080
0.000	0.049	0.078	0.195	0.081
0.000	0.050	0.078	0.196	0.080

Number of Simulators Used: 5

Remarks:
N/A

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL

Signature and Printed Name

12/11/2023
Date

Florida Department of Law Enforcement

Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 14:23

Date of Inspection: 11/19/2023

Serial Number: 80-000759
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.049	0.078	0.196	0.080
0.000	0.049	0.079	0.196	0.081
0.000	0.049	0.078	0.196	0.081

Number of Simulators Used: 5

Remarks:
N/A

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Signature and Printed Name
NEIL F RUBEL

11/19/2023
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 23:56

Date of Inspection: 10/17/2023

Serial Number: 80-000759
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.048	0.078	0.195	0.080
0.000	0.049	0.078	0.196	0.080
0.000	0.050	0.079	0.195	0.079

Number of Simulators Used: 5

Remarks:

N/A



The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


Signature and Printed Name

NEIL F RUBEL

10/17/2023
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 07:11

Date of Inspection: 09/21/2023

Serial Number: 80-000759
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.048	0.078	0.195	0.080
0.000	0.049	0.078	0.195	0.079
0.000	0.048	0.079	0.195	0.080


Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

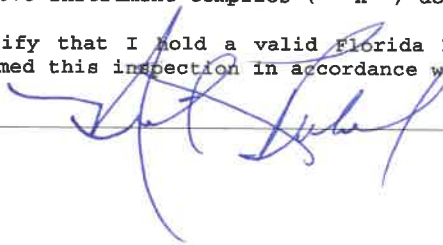
Signature and Printed Name

09/21/2023
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 13:21

Date of Inspection: 08/16/2023

Serial Number: 80-000759
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.048	0.079	0.198	0.082
0.000	0.048	0.078	0.197	0.081
0.000	0.048	0.078	0.198	0.081

Number of Simulators Used: 5

Remarks:
N/A

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

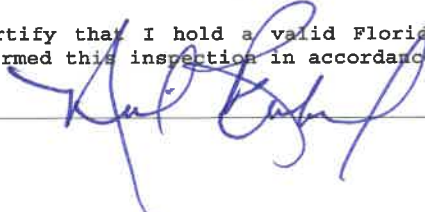
NEIL F RUBEL
Signature and Printed Name

08/16/2023
Date

Florida Department of Law Enforcement

Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 14:43

Date of Inspection: 06/20/2023

Serial Number: 80-000759
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.049	0.078	0.196	0.080
0.000	0.049	0.078	0.196	0.079
0.000	0.049	0.078	0.197	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



NICHOLAS M LITTLE

Signature and Printed Name

06/20/2023
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 15:06

Date of Inspection: 05/01/2023

Serial Number: 80-000759
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.049 / 0.049	0.079	0.199	0.084
0.000	0.049 / 0.049	0.080	0.199	0.084
0.000	0.049 / 0.049	0.081	0.198	0.083

Number of Simulators Used: 5

Remarks:

05: RFI Detect CELL PHONE ACTIVATION/REMOVED.

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL

Signature and Printed Name

05/01/2023
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 23:25

Date of Inspection: 04/08/2023

Serial Number: 80-000759
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.048	0.078	0.197	0.081
0.000	0.048	0.079	0.198	0.080
0.000	0.048	0.079	0.198	0.080


Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

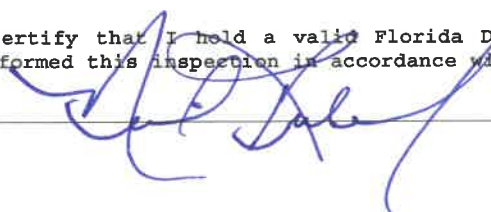
Signature and Printed Name

NEIL F RUBEL

04/08/2023
Date

After Annual Insp

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 13:18

Date of Inspection: 01/12/2023

Serial Number: 80-000759
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.049	0.077	0.196	0.080
0.000	0.049	0.078	0.197	0.080
0.000	0.049	0.078	0.196	0.080

Number of Simulators Used: 5

Remarks:
NA

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

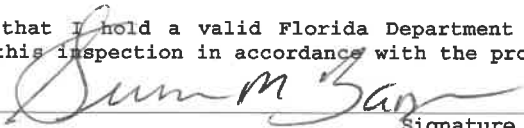

SUSAN M BARGE

Signature and Printed Name

01/12/2023
Date

Before Annual
Inspr.

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 11:40

Date of Inspection: 01/04/2023

Serial Number: 80-000759
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.048	0.078	0.196	0.079
0.000	0.048	0.079	0.196	0.080
0.000	0.048	0.079	0.197	0.080


Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

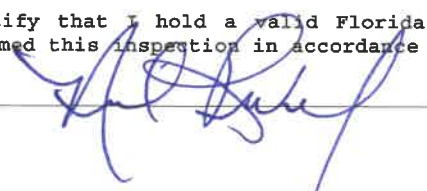
Signature and Printed Name

NEIL F RUBEL

01/04/2023
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 11:56

Date of Inspection: 02/16/2023

Serial Number: 80-000759
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	
	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.048	0.078	0.188 / 0.193	0.080
0.000	0.048	0.078	0.191 / 0.195	0.080
0.000	0.048	0.078	0.192 / 0.197	0.080


Number of Simulators Used: 5

Remarks:

20: Control Outside Tolerance. TIGHTEN LID

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

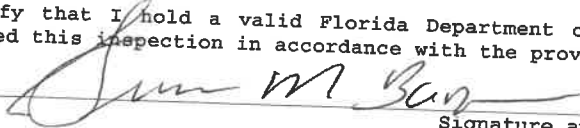

Signature and Printed Name

SUSAN M BARGE

02/16/2023
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 09:39

Date of Inspection: 03/06/2023

Serial Number: 80-000759
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.047	0.076	0.195	0.079
0.000	0.047	0.077	0.195	0.079
0.000	0.048	0.077	0.196	0.079


Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

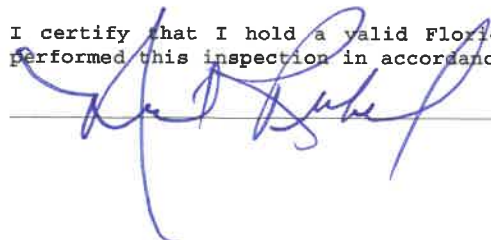

NEIL F RUBEL
Signature and Printed Name

03/06/2023
Date