

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP  
Time of Inspection: 11:55

Date of Inspection: 12/02/2023

Serial Number: 80-000781  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.048	0.078	0.197	0.080
0.000	0.048	0.078	0.199	0.080
0.000	0.049	0.079	0.200	0.079

Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL

Signature and Printed Name

12/02/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 23:31

Date of Inspection: 11/28/2023

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.049	0.078	0.192	0.081
0.000	0.049	0.078	0.193	0.081
0.000	0.049	0.078	0.193	0.081

Number of Simulators Used: 5


Remarks:

N/A



The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

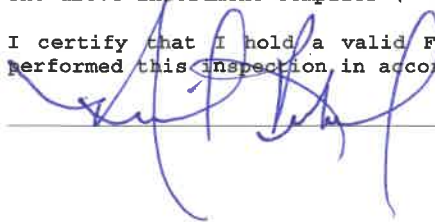

NEIL F RUBEL  
Signature and Printed Name

11/28/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 23:50

Date of Inspection: 10/17/2023

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.049	0.077	0.197	0.080
0.000	0.050	0.078	0.198	0.080
0.000	0.050	0.079	0.199	0.080

Number of Simulators Used: 5


Remarks:

N/A



The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

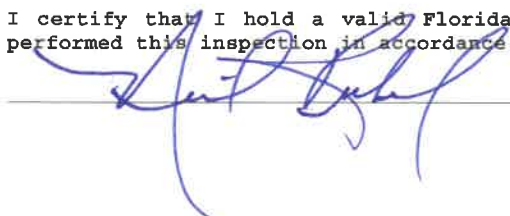

NEIL F RUBEL

Signature and Printed Name

10/17/2023

Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 10:54

Date of Inspection: 09/27/2023

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.049	0.077	0.196	0.080
0.000	0.049	0.077	0.197	0.080
0.000	0.049	0.077	0.197	0.080

Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL

Signature and Printed Name

09/27/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 10:13

Date of Inspection: 08/13/2023

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.048	0.079	0.197	0.080
0.000	0.049	0.080	0.198	0.079
0.000	0.049	0.081	0.200	0.079

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
 \_\_\_\_\_  
 Signature and Printed Name

NEIL F RUBEL

08/13/2023  
 Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 13:52

Date of Inspection: 06/26/2023

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.048	0.079	0.198	0.080
0.000	0.049	0.079	0.200	0.079
0.000	0.050	0.079	0.201	0.080

Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL  
Signature and Printed Name

06/26/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 10:55

Date of Inspection: 05/01/2023

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.048	0.079	0.198	0.080
0.000	0.048	0.080	0.199	0.080
0.000	0.049	0.080	0.200	0.080

Number of Simulators Used: 5

Remarks:

N/A  
*NR*

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL

Signature and Printed Name

05/01/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP  
Time of Inspection: 15:28

Date of Inspection: 04/26/2023

Serial Number: 80-000781  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.047	0.078	0.197	0.080
0.000	0.048	0.078	0.197	0.080
0.000	0.048	0.078	0.197	0.079

Number of Simulators Used: 5

Remarks:

N/A 

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL

Signature and Printed Name

04/26/2023  
Date



After Annual Insp

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 10:35

Date of Inspection: 01/25/2023

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.049	0.076	0.194	0.081
0.000	0.049	0.077	0.197	0.080
0.000	0.049	0.077	0.197	0.080

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

SUSAN M BARGE

Signature and Printed Name

01/25/2023  
Date

Before Annual Insp

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 13:20

Date of Inspection: 01/17/2023

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.048	0.078	0.197	0.081
0.000	0.049	0.078	0.198	0.080
0.000	0.049	0.078	0.197	0.080

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

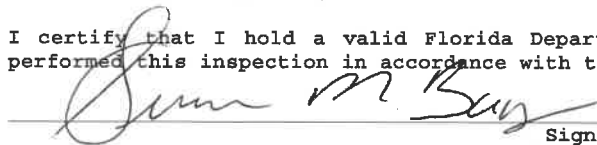

SUSAN M BARGE

Signature and Printed Name

01/17/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 15:08

Date of Inspection: 02/08/2023

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.048	0.079	0.198	0.080
0.000	0.049	0.079	0.198	0.080
0.000	0.049	0.079	0.198	0.080

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

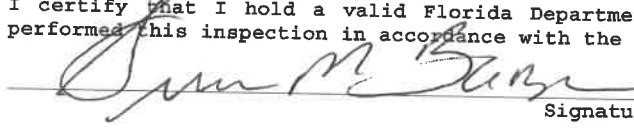  
 \_\_\_\_\_  
 Signature and Printed Name

SUSAN M BARGE

02/08/2023  
 Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 12:49

Date of Inspection: 03/07/2023

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1482048 Exp: 04/21/2024
0.000	0.047	0.077	0.195	0.080
0.000	0.049	0.078	0.197	0.080
0.000	0.049	0.078	0.197	0.079

Number of Simulators Used: 5


Remarks:

N/A



The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

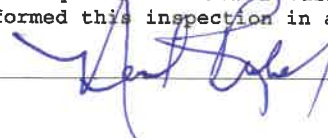  
 \_\_\_\_\_  
 Signature and Printed Name

NEIL F RUBEL

03/07/2023  
 Date