

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 13:18

Date of Inspection: 07/17/2023

Serial Number: 80-000968

Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |


| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202108D<br>Exp: 08/17/2023 | 0.20g/210L Test (g/210L)<br>Lot#:202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:402330433<br>Exp: 01/24/2025 |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|----------------------------------------------------------------------------|
| 0.000                      | 0.048                                                       | 0.076                                                       | 0.195                                                       | 0.079                                                                      |
| 0.000                      | 0.047                                                       | 0.077                                                       | 0.196                                                       | 0.079                                                                      |
| 0.000                      | 0.048                                                       | 0.078                                                       | 0.195                                                       | 0.080                                                                      |

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

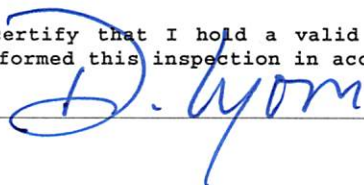

DANIEL E LYONS

Signature and Printed Name

07/17/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Serial Number: 80-000968

Time of Inspection: 14:30

Date of Inspection: 06/21/2023

Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |


| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202108D<br>Exp: 08/17/2023 | 0.20g/210L Test (g/210L)<br>Lot#:202106B<br>Exp: 06/22/2023 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:402330433<br>Exp: 01/24/2025 |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|----------------------------------------------------------------------------|
| 0.000                      | 0.047                                                       | 0.076                                                       | 0.194                                                       | 0.080                                                                      |
| 0.000                      | 0.047                                                       | 0.076                                                       | 0.195                                                       | 0.080                                                                      |
| 0.000                      | 0.048                                                       | 0.077                                                       | 0.195                                                       | 0.080                                                                      |

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

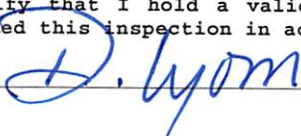

DANIEL E LYONS

Signature and Printed Name

06/21/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 12:24

Date of Inspection: 05/19/2023

Serial Number: 80-000968

Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |


| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202108D<br>Exp: 08/17/2023 | 0.20g/210L Test (g/210L)<br>Lot#:202106B<br>Exp: 06/22/2023 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:402330433<br>Exp: 01/24/2025 |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|----------------------------------------------------------------------------|
| 0.000                      | 0.048                                                       | 0.077                                                       | 0.195                                                       | 0.079                                                                      |
| 0.000                      | 0.048                                                       | 0.077                                                       | 0.195                                                       | 0.080                                                                      |
| 0.000                      | 0.048                                                       | 0.077                                                       | 0.194                                                       | 0.080                                                                      |

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

05/19/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 14:22

Date of Inspection: 04/25/2023

Serial Number: 80-000968

Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |


| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202108D<br>Exp: 08/17/2023 | 0.20g/210L Test (g/210L)<br>Lot#:202106B<br>Exp: 06/22/2023 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:402330422<br>Exp: 01/24/2025 |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|----------------------------------------------------------------------------|
| 0.000                      | 0.047                                                       | 0.078                                                       | 0.195                                                       | 0.080                                                                      |
| 0.000                      | 0.047                                                       | 0.078                                                       | 0.195                                                       | 0.080                                                                      |
| 0.000                      | 0.047                                                       | 0.078                                                       | 0.195                                                       | 0.081                                                                      |

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
 \_\_\_\_\_  
 Signature and Printed Name DANIEL E LYONS  
 04/25/2023  
 Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Serial Number: 80-000968

Time of Inspection: 11:01

Date of Inspection: 03/24/2023

Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202108D<br>Exp: 08/17/2023 | 0.20g/210L Test (g/210L)<br>Lot#:202106B<br>Exp: 06/22/2023 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:402330433<br>Exp: 01/24/2025 |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|----------------------------------------------------------------------------|
| 0.000                      | 0.049                                                       | 0.078                                                       | 0.198                                                       | 0.000 / 0.080                                                              |
| 0.000                      | 0.049                                                       | 0.078                                                       | 0.198                                                       | 0.000 / 0.080                                                              |
| 0.000                      | 0.049                                                       | 0.078                                                       | 0.199                                                       | 0.000 / 0.080                                                              |

Number of Simulators Used: 5

**Remarks:**

08:Cntl Out Tol, DID NOT CONNECT DRY GAS LINE  
ITHIN COMPLIANCE

. DRY GAS LINE CONN, REITESTED, RE-TEST W

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 DANIEL/OWEN E LYONS/GAYLE  
Signature and Printed Name

03/24/2023  
Date