



Florida Department of
Law Enforcement

AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Davie PD

Instrument Serial Number: 80-001056

AGENCY INSPECTION DISCREPENCY

Agency Inspector: David Haines

Inspection Date: 07/26/2023

☐ A test was repeated without reason for repeat or the corrective action given

☐ Alcohol Free/Mouth Alcohol ☐ Alcohol Free Test ☐ Interferent Detect

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Agency Inspection not conducted for calendar month

☐ Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ Lot Number and/or Expiration Date for Standards entered incorrectly

☒ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ Other Electronic Data Review/Comments: The 0.05 lot number is missing a digit.

REQUESTED CORRECTIVE ACTION

☒ Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector

☐ Provide written explanation regarding referenced item(s) to Department Inspector

☐ Remove instrument from evidentiary use until otherwise directed by the Department

☐ Other:

Taylor Gutschow

Digitally signed by Taylor

Gutschow

Date: 2023.10.30 13:13:10 -04'00'

10/30/2023

Signature of Alcohol Testing Program Staff Member

Date

Amended 11/4/23

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: DAVIE PD

Time of Inspection: 12:30

Date of Inspection: 07/26/2023

Serial Number: 80-001056

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

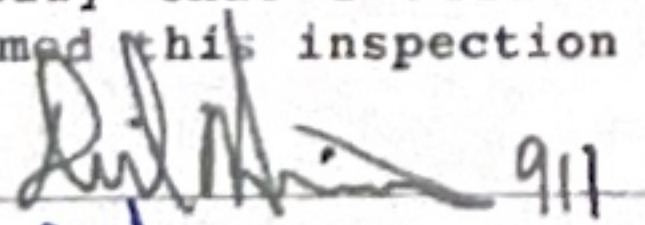
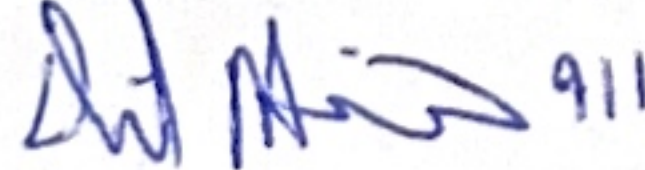
Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) 20211A 202112A Lot#: 20211A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#: 202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#: 202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 1497672 Exp: 05/20/2024
0.000	0.051	0.081	0.203	0.080
0.000	0.051	0.081	0.203	0.080
0.000	0.052	0.082	0.204	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


911

911

DAVID K HAINES
Signature and Printed Name

07/26/2023
Date



Florida Department of
Law Enforcement

AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Davie PD

Instrument Serial Number: 80-001056

AGENCY INSPECTION DISCREPENCY

Agency Inspector: David Haines

Inspection Date: 09/12/2023

☒ **A test was repeated without reason for repeat or the corrective action given**

☐ Alcohol Free/Mouth Alcohol ☒ Alcohol Free Test ☐ Interferent Detect

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ **Agency Inspection not conducted for calendar month**

☐ **Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection**

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ **Lot Number and/or Expiration Date for Standards entered incorrectly**

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ **Other Electronic Data Review/Comments:** The Alcohol-Free Test was repeated. Please include a remark describing the corrective action taken prior to repeating the test.

REQUESTED CORRECTIVE ACTION

☒ **Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector**

☐ **Provide written explanation regarding referenced item(s) to Department Inspector**

☐ **Remove instrument from evidentiary use until otherwise directed by the Department**

☐ **Other:**

Taylor Gutschow

Digitally signed by Taylor

Gutschow

Date: 2023.11.13 10:23:10 -05'00'

11/13/2023

Signature of Alcohol Testing Program Staff Member

Date

Amended 11/20/2023

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: DAVIE PD

Time of Inspection: 12:05

Date of Inspection: 09/12/2023

Serial Number: 80-001056

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1497672 Exp: 05/20/2024
/ 0.000	0.051	0.081	0.204	0.079
/ 0.000	0.051	0.082	0.204	0.079
/ 0.000	0.051	0.081	0.204	0.079

Number of Simulators Used: 5

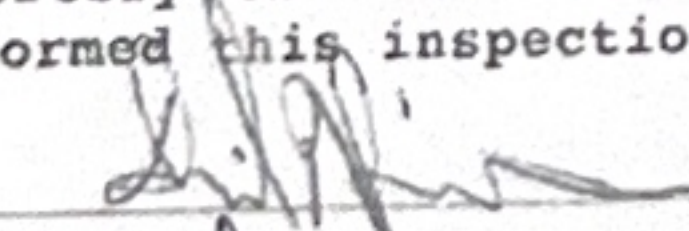
Remarks:

00: Ambient Fail.

Cleared mouth of mouth alcohol & successfully retested Alcohol-Free test

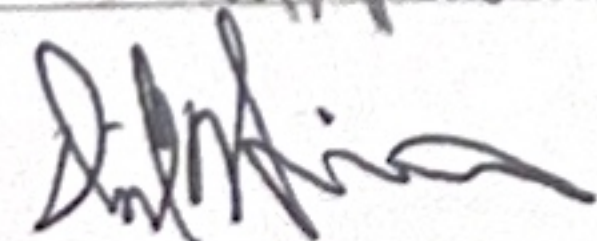
The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DAVID K HAINES

Signature and Printed Name

 11/20/23

09/12/2023
Date