

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO
Time of Inspection: 10:15

Date of Inspection: 11/06/2023

Serial Number: 80-006236
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:402558895 Exp: 10/03/2025	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:
0.000	0.050	0.000 / 0.000		
0.000	0.050	0.000 / 0.000		
0.000	0.050	0.000 / 0.000		

Number of Simulators Used: 5


Remarks:

08: Control Outside Tolerance, Control Outside Tolerance. Non-compliance: CONTROL OUTSIDE TOLERANCE
.08 DGS.

Note: Upon inspection .08 Reference Solution was accidentally skipped. Contacted FDLE who advised to re-run entire inspection - was

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

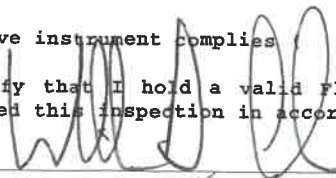

WILLIAM COLEMAN

Signature and Printed Name

11/06/2023
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: **MANATEE COUNTY SO**
Time of Inspection: **13:59**

Date of Inspection: **11/06/2023**

Serial Number: **80-006236**
Software: **8100.27**

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402558895 Exp: 10/03/2025
0.000	0.050	0.079	0.199	0.080
0.000	0.050	0.079	0.199	0.080
0.000	0.050	0.079	0.199	0.079


Number of Simulators Used: 5

Remarks:

Re-inspection after .08 Reference Solution was accidentally skipped.
Per Dept. Inspector, re-inspection was authorized.

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

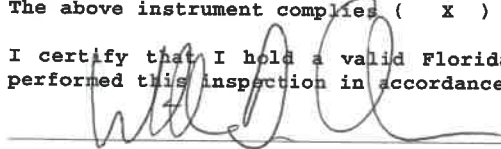

WILLIAM COLEMAN
Signature and Printed Name

11/06/2023
Date



Florida Department of
Law Enforcement

AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Manatee CSO

Instrument Serial Number: 80-006236

AGENCY INSPECTION DISCREPENCY

Agency Inspector: William Coleman

Inspection Date: 07/20/2023

☒ **A test was repeated without reason for repeat or the corrective action given**

- ☐ Alcohol Free/Mouth Alcohol ☐ Alcohol Free Test ☒ Interferent Detect
☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ **Agency Inspection not conducted for calendar month**

☐ **Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection**

- ☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ **Lot Number and/or Expiration Date for Standards entered incorrectly**

- ☒ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ **Other Electronic Data Review/Comments:** The 0.05 lot number is mistyped. A remark describing the corrective action (RFI Detect) on the Interferent Detect Test must be included.

REQUESTED CORRECTIVE ACTION

- ☒ **Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector**
- ☐ **Provide written explanation regarding referenced item(s) to Department Inspector**
- ☐ **Remove instrument from evidentiary use until otherwise directed by the Department**
- ☐ **Other:**

Taylor Gutschow

Digitally signed by Taylor
Gutschow
Date: 2023.10.30 13:21:29 -04'00'

Signature of Alcohol Testing Program Staff Member

10/30/2023

Date

Amended
10-31-2023

WDC

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO
Time of Inspection: 09:50

Date of Inspection: 07/20/2023

Serial Number: 80-006236
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) 202303J Lot#: 20220625 Exp: 03/28/2025 WDC	0.08g/210L Test (g/210L) Lot#: 202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#: 202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 402558895 Exp: 10/03/2025
0.000	0.049	0.079	0.197	0.079
0.000	0.049	0.079	0.198	0.079
0.000	0.049	0.079	0.197	0.078

Number of Simulators Used: 5

Remarks:

Int Det: RFI Detect.

202303J


WDC

INT DET

- WDC - RFI Source located conducted test 2nd time.
- WDC - .05 Reference Solution wrong Lot # entered by mistake.

The above instrument complies (☒) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

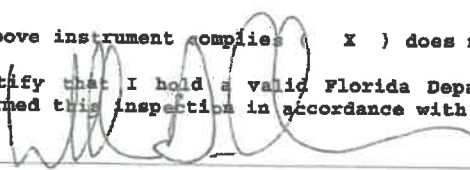

WILLIAM D COLEMAN

Signature and Printed Name

07/20/2023
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO

Time of Inspection: 13:40

Date of Inspection: 06/12/2023

Serial Number: 80-006236

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/14/2024 <i>WDC</i> <i>06/15/2024</i>	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402558895 Exp: 10/03/2025
0.000	0.049	0.079	0.198	0.079
0.000	0.049	0.079	0.199	0.079
0.000	0.049	0.079	0.199	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 WILLIAM COLEMAN
Signature and Printed Name

06/12/2023
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO
Time of Inspection: 09:50

Date of Inspection: 07/20/2023

Serial Number: 80-006236
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) 2023035 Lot#: 2022035 WDL Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#: 202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#: 202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 402558895 Exp: 10/03/2025
0.000	0.049	0.079	0.197	0.079
0.000	0.049	0.079	0.198	0.079
0.000	0.049	0.079	0.197	0.078

Number of Simulators Used: 5


Remarks:

Int Det: RFI Detect.

- RFI Source located conducted test 2nd time.
- .05 Reference Solution wrong Lot # entered by mistake.

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

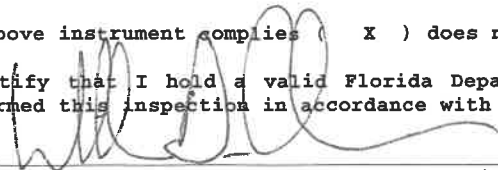

WILLIAM D COLEMAN

Signature and Printed Name

07/20/2023
Date



Florida Department of
Law Enforcement

AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Manatee CSO

Instrument Serial Number: 80-006236

AGENCY INSPECTION DISCREPENCY

Agency Inspector: William Coleman

Inspection Date: 02/06/2023

☐ A test was repeated without reason for repeat or the corrective action given

☐ Alcohol Free/Mouth Alcohol ☐ Alcohol Free Test ☐ Interferent Detect

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Agency Inspection not conducted for calendar month

☐ Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ Lot Number and/or Expiration Date for Standards entered incorrectly

☐ 0.050 g/210L ☐ 0.080 g/210L ☒ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Other Electronic Data Review/Comments:

REQUESTED CORRECTIVE ACTION

☒ Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector

☐ Provide written explanation regarding referenced item(s) to Department Inspector

☐ Remove instrument from evidentiary use until otherwise directed by the Department

☐ Other:

Taylor Gutschow

Digitally signed by Taylor

Gutschow

Date: 2023.05.17 09:18:33 -04'00'

05/17/2023

Signature of Alcohol Testing Program Staff Member

Date

Amended
Florida Department of Law Enforcement
Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO
Time of Inspection: 14:49

Date of Inspection: 02/06/2023

Serial Number: 80-006236
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) <i>202106B</i> Lot#:201205B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402357111 Exp: 02/10/2025
0.000	0.050	0.079	0.198	0.080
0.000	0.049	0.079	0.198	0.080
0.000	0.050	0.079	0.198	0.080


Number of Simulators Used: 5

Remarks:

Incorrect Lot # entered. Corrected above (WOC)

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

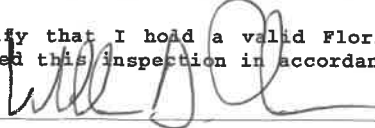

WILLIAM COLEMAN

Signature and Printed Name

02/06/2023
Date