

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 15:00

Date of Inspection: 12/11/2023

Serial Number: 80-006760  
Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202303J<br>Exp: 03/28/2025 | 0.08g/210L Test (g/210L)<br>Lot#:202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#:202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:402477284<br>Exp: 06/27/2025 |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|----------------------------------------------------------------------------|
| 0.000                      | 0.048                                                       | 0.078                                                       | 0.196                                                       | 0.080                                                                      |
| 0.000                      | 0.049                                                       | 0.079                                                       | 0.195                                                       | 0.080                                                                      |
| 0.000                      | 0.049                                                       | 0.079                                                       | 0.195                                                       | 0.080                                                                      |

Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies ( X ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL

Signature and Printed Name

12/11/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 14:17

Date of Inspection: 11/19/2023

Serial Number: 80-006760  
Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

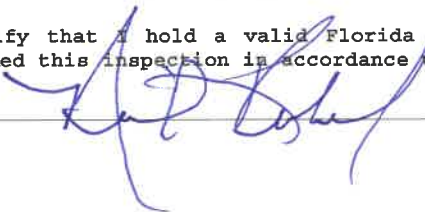
|                            |                                                             |                                                             |                                                             |                                                                            |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|----------------------------------------------------------------------------|
| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#:202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:402477284<br>Exp: 06/27/2025 |
| 0.000                      | 0.048                                                       | 0.077                                                       | 0.192                                                       | 0.080                                                                      |
| 0.000                      | 0.047                                                       | 0.077                                                       | 0.193                                                       | 0.080                                                                      |
| 0.000                      | 0.048                                                       | 0.077                                                       | 0.194                                                       | 0.080                                                                      |

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies ( X ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
Signature and Printed Name

NEIL F RUBEL

11/19/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL

Time of Inspection: 07:31

Date of Inspection: 09/21/2023

Serial Number: 80-006760

Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

|                            |                                                             |                                                             |                                                             |                                                                             |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-----------------------------------------------------------------------------|
| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#:202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:2402477284<br>Exp: 06/27/2025 |
| 0.000                      | 0.048                                                       | 0.077                                                       | 0.194                                                       | 0.080                                                                       |
| 0.000                      | 0.048                                                       | 0.077                                                       | 0.195                                                       | 0.080                                                                       |
| 0.000                      | 0.049                                                       | 0.077                                                       | 0.195                                                       | 0.080                                                                       |

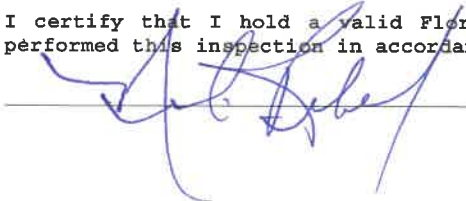
Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies ( X ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
Signature and Printed Name

NEIL F RUBEL

09/21/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 10:27

Date of Inspection: 08/13/2023

Serial Number: 80-006760  
Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

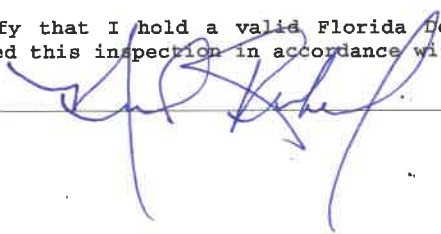
|                            |                                                             |                                                             |                                                             |                                                                             |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-----------------------------------------------------------------------------|
| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#:202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:2402477284<br>Exp: 06/27/2025 |
| 0.000                      | 0.048                                                       | 0.078                                                       | 0.195                                                       | 0.079                                                                       |
| 0.000                      | 0.048                                                       | 0.078                                                       | 0.196                                                       | 0.079                                                                       |
| 0.000                      | 0.048                                                       | 0.078                                                       | 0.196                                                       | 0.080                                                                       |

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies ( X ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
NEIL F RUBEL  
Signature and Printed Name

08/13/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 07:27

Date of Inspection: 06/21/2023

Serial Number: 80-006760  
Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#:202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:2402477284<br>Exp: 06/27/2025 |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-----------------------------------------------------------------------------|
| 0.000                      | 0.047                                                       | 0.077                                                       | 0.196                                                       | 0.077                                                                       |
| 0.000                      | 0.047                                                       | 0.078                                                       | 0.196                                                       | 0.078                                                                       |
| 0.000                      | 0.047                                                       | 0.078                                                       | 0.196                                                       | 0.078                                                                       |

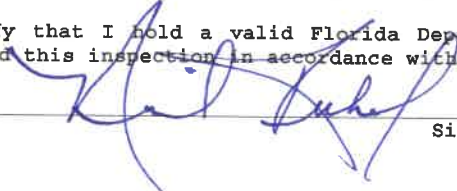
Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
Signature and Printed Name

NEIL F RUBEL

06/21/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 07:27

Date of Inspection: 06/21/2023

Serial Number: 80-006760  
Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#:202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:2402477284<br>Exp: 06/27/2025 |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-----------------------------------------------------------------------------|
| 0.000                      | 0.047                                                       | 0.077                                                       | 0.196                                                       | 0.077                                                                       |
| 0.000                      | 0.047                                                       | 0.078                                                       | 0.196                                                       | 0.078                                                                       |
| 0.000                      | 0.047                                                       | 0.078                                                       | 0.196                                                       | 0.078                                                                       |

Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies ( X ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Signature and Printed Name NEIL F RUBEL

06/21/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 13:27

Date of Inspection: 05/10/2023

Serial Number: 80-006760  
Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

|                            |                                                             |                                                             |                                                             |                                                                             |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-----------------------------------------------------------------------------|
| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#:202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:2402477284<br>Exp: 06/27/2025 |
| 0.000                      | 0.048                                                       | 0.077                                                       | 0.199                                                       | 0.080                                                                       |
| 0.000                      | 0.048                                                       | 0.078                                                       | 0.200                                                       | 0.080                                                                       |
| 0.000                      | 0.049                                                       | 0.079                                                       | 0.199                                                       | 0.080                                                                       |

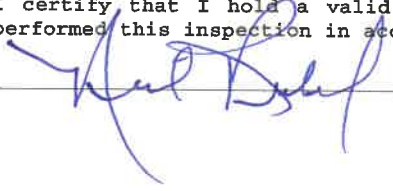
Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies ( X ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
Signature and Printed Name

NEIL F RUBEL

05/10/2023  
Date

# Florida Department of Law Enforcement

## Alcohol Testing Program

### AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 03:25

Date of Inspection: 04/04/2023

Serial Number: 80-006760  
Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#:202106B<br>Exp: 06/22/2023 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:1327124<br>Exp: 05/14/2023 |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|--------------------------------------------------------------------------|
| 0.000                      | 0.046                                                       | 0.078                                                       | 0.193                                                       | 0.079                                                                    |
| 0.000                      | 0.046                                                       | 0.078                                                       | 0.193                                                       | 0.079                                                                    |
| 0.000                      | 0.046                                                       | 0.078                                                       | 0.194                                                       | 0.079                                                                    |

Number of Simulators Used: 5

Remarks:

N/A

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL

Signature and Printed Name

04/04/2023

Date

# Florida Department of Law Enforcement Alcohol Testing Program

*After Annual Insp*

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 13:04

Date of Inspection: 01/12/2023

Serial Number: 80-006760  
Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202108D<br>Exp: 08/17/2023 | 0.20g/210L Test (g/210L)<br>Lot#:202106B<br>Exp: 06/22/2023 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:1327124<br>Exp: 05/14/2023 |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|--------------------------------------------------------------------------|
| 0.000                      | 0.044 / 0.048                                               | 0.074 / 0.078                                               | 0.190                                                       | 0.079                                                                    |
| 0.000                      | 0.047 / 0.049                                               | 0.077 / 0.079                                               | 0.194                                                       | 0.078                                                                    |
| 0.000                      | 0.048 / 0.049                                               | 0.078 / 0.079                                               | 0.196                                                       | 0.079                                                                    |

Number of Simulators Used: 5

**Remarks:**

05: Control Outside Tolerance. 08: Control Outside Tolerance. OUTSIDE CONTROL TOLERANCE .05 .08 TIGHT EN LID

*sm3*

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

*Susan M Barge* SUSAN M BARGE  
Signature and Printed Name

01/12/2023  
Date

Before Annual Insp

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 11:51

Date of Inspection: 01/04/2023

Serial Number: 80-006760

Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

|                            |                                                             |                                                             |                                                             |                                                                          |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|--------------------------------------------------------------------------|
| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202108D<br>Exp: 08/17/2023 | 0.20g/210L Test (g/210L)<br>Lot#:202106B<br>Exp: 06/22/2023 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:1327124<br>Exp: 05/14/2023 |
| 0.000                      | 0.047                                                       | 0.078                                                       | 0.193                                                       | 0.078                                                                    |
| 0.000                      | 0.048                                                       | 0.078                                                       | 0.194                                                       | 0.078                                                                    |
| 0.000                      | 0.048                                                       | 0.078                                                       | 0.194                                                       | 0.078                                                                    |

Number of Simulators Used: 5

Remarks:

N/A

NR

The above instrument complies ( X ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

NEIL F RUBEL

Signature and Printed Name

01/04/2023

Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 11:57

Date of Inspection: 02/16/2023

Serial Number: 80-006760  
Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     |    |
| Diagnostic Check (Pre-Inspection): OK       |     | No |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

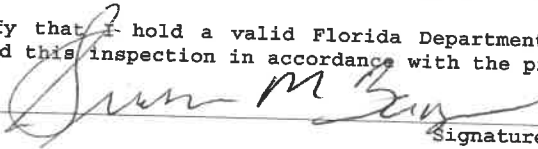
| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202108D<br>Exp: 08/17/2023 | 0.20g/210L Test (g/210L)<br>Lot#:202106B<br>Exp: 06/22/2023 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:1327124<br>Exp: 05/14/2023 |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|--------------------------------------------------------------------------|
| 0.000                      | 0.045                                                       | 0.075                                                       | 0.192                                                       | 0.079                                                                    |
| 0.000                      | 0.047                                                       | 0.077                                                       | 0.195                                                       | 0.079                                                                    |
| 0.000                      | 0.047                                                       | 0.078                                                       | 0.195                                                       | 0.079                                                                    |

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE  
Signature and Printed Name

02/16/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 09:26

Date of Inspection: 03/06/2023

Serial Number: 80-006760  
Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

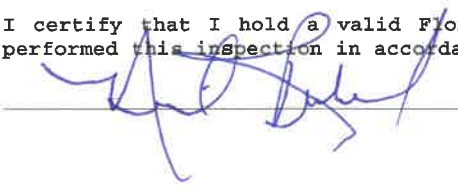
|                            |                                                             |                                                             |                                                             |                                                                          |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|--------------------------------------------------------------------------|
| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#:202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:1327124<br>Exp: 05/14/2023 |
| 0.000                      | 0.047                                                       | 0.076                                                       | 0.200                                                       | 0.077                                                                    |
| 0.000                      | 0.046                                                       | 0.076                                                       | 0.197                                                       | 0.077                                                                    |
| 0.000                      | 0.046                                                       | 0.076                                                       | 0.196                                                       | 0.077                                                                    |

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies ( X ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
Signature and Printed Name

NEIL F RUBEL

03/06/2023  
Date