

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: Broward County SO

Serial Number: 80-006925

Time of Inspection:

Date of Inspection: July 2023

Software: 8100.27

CHECK OR TEST	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		
Alcohol Free Subject Test: 0.000		
Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect		
Diagnostic Check (Post-Inspection): OK		


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Number of Simulators Used: _____

Remarks: Inspection was not conducted as the instrument was sent to CMI, Inc for repairs.

The above instrument complies (____) does not comply (____) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

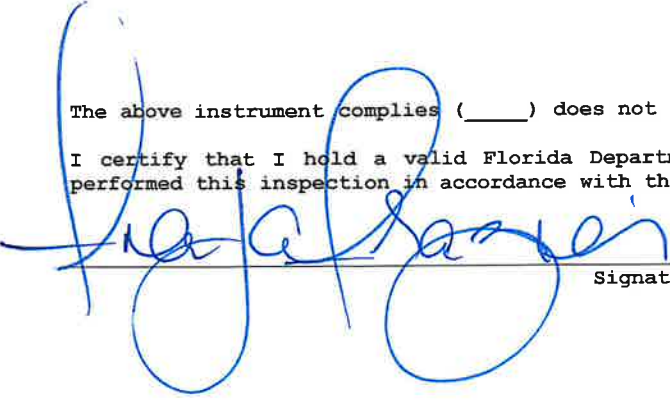
Signature and Printed Name

07/05/2023
Date



Florida Department of
Law Enforcement

**AGENCY INSPECTION AND OTHER
ELECTRONIC DATA REVIEW**

Agency: Broward CSO

Instrument Serial Number: 80-006925

AGENCY INSPECTION DISCREPENCY

Agency Inspector: Anaya Frazier

Inspection Date: 01/04/2023

☒ **A test was repeated without reason for repeat or the corrective action given**

- ☐ Alcohol Free/Mouth Alcohol ☐ Alcohol Free Test ☐ Interferent Detect
☒ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ **Agency Inspection not conducted for calendar month**

☐ **Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection**

- ☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ **Lot Number and/or Expiration Date for Standards entered incorrectly**

- ☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ **Other Electronic Data Review/Comments:**

REQUESTED CORRECTIVE ACTION

☒ **Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector**

☐ **Provide written explanation regarding referenced item(s) to Department Inspector**

☐ **Remove instrument from evidentiary use until otherwise directed by the Department**

☐ **Other:**

Taylor Gutschow

Digitally signed by Taylor

Gutschow

Date: 2023.05.17 11:10:08 -04'00'

05/17/2023

Signature of Alcohol Testing Program Staff Member

Date

Amendment II

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: BROWARD COUNTY SO
Time of Inspection: 13:07

Date of Inspection: 01/04/2023

Serial Number: 80-006925
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402477283 Exp: 06/24/2025
0.000	0.044 / 0.051	0.078	0.200	0.077
0.000	0.048 / 0.050	0.078	0.202	0.077
0.000	0.048 / 0.049	0.081	0.202	0.078

Number of Simulators Used: 5

Remarks:

05: Control Outside Tolerance.JGUZMAN IN TRAINING

Control Outside Tolerance. Unknown Reason. Instrument was within tolerance on sample 2 and 3 of the first test. And all 3 samples were in tolerance on the Repeat Test. 04 5/20/2023

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

[Signature]

ANAYA S FRAZIER

Signature and Printed Name

01/04/2023
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT – INTOXILYZER 8000

Agency: Broward County SO

Serial Number: 80-006925

Time of Inspection:

Date of Inspection: June 2023

Software: 8100.27

CHECK OR TEST	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		
Alcohol Free Subject Test: 0.000		
Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect		
Diagnostic Check (Post-Inspection): OK		

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Number of Simulators Used: _____

Remarks: Inspection was not conducted as the instrument was sent to CMI, Inc for repairs.

The above instrument complies (____) does not comply (____) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


Signature and Printed Name

06/07/2023
Date

Florida Department of Law Enforcement

Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: Broward County SO

Time of Inspection:

Software: 8100.27

Serial Number: 80-006925

Date of Inspection: April 2023

CHECK OR TEST	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		
Alcohol Free Subject Test: 0.000		
Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect		
Diagnostic Check (Post-Inspection): OK		


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Number of Simulators Used: _____

Remarks: Inspection was not conducted as the instrument was sent to CMI, Inc for repairs.

The above instrument complies (____) does not comply (____) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

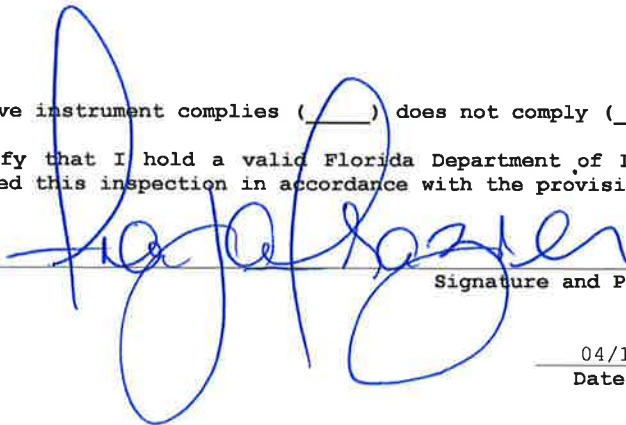

Signature and Printed Name

04/12/2023

Date

Florida Department of Law Enforcement

Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: Broward County SO

Serial Number: 80-006925

Time of Inspection:

Date of Inspection: May 2023

Software: 8100.27

CHECK OR TEST	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		
Alcohol Free Subject Test: 0.000		
Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect		
Diagnostic Check (Post-Inspection): OK		


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Number of Simulators Used: _____

Remarks: Inspection was not conducted as the instrument was sent to CMI, Inc for repairs.

The above instrument complies (____) does not comply (____) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

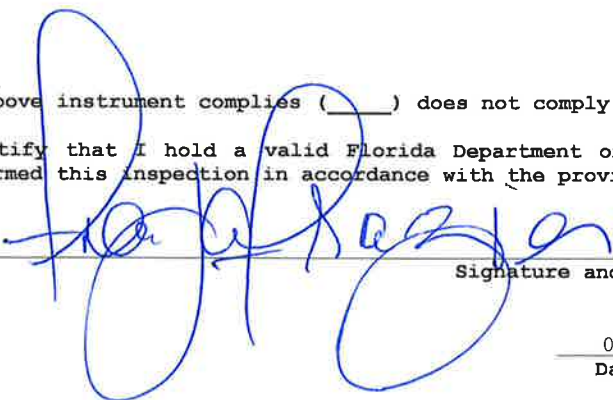

Signature and Printed Name

05/03/2023

Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: Broward County SO

Serial Number: 80-006925

Time of Inspection:

Date of Inspection: March 2023

Software: 8100.27

CHECK OR TEST	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		
Alcohol Free Subject Test: 0.000		
Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect		
Diagnostic Check (Post-Inspection): OK		

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Number of Simulators Used: _____

Remarks: Inspection was not conducted as the instrument was sent to CMI, Inc for repairs.

The above instrument complies (____) does not comply (____) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


Signature and Printed Name

03/11/2023
Date