








INSTRUMENT PROCESSING SHEET

Agency Fort Lauderdale PDS/N 80-007009Florida Department of
Law EnforcementDate In 08/17/2023DI Completion Date 08/21/2023☒ Ship ☐ P/U ☐ H/D ☐ CMI ☐ EE

Intake	By TDG	Quality Checks	By TDG	Date 08/21/2023	Flow Calibration	By	Date																																							
<input checked="" type="checkbox"/> Annual <input type="checkbox"/> Registration <input checked="" type="checkbox"/> Return from CMI / EE Visual Inspection: <input checked="" type="checkbox"/> Case <input checked="" type="checkbox"/> Handle <input checked="" type="checkbox"/> Keyboard <input checked="" type="checkbox"/> Dry Gas Shelf <input checked="" type="checkbox"/> Feet <input checked="" type="checkbox"/> Breath Tube <input checked="" type="checkbox"/> Ports <input checked="" type="checkbox"/> Screws Tight Other Equipment/ Accessories: <input type="checkbox"/> Power cord <input type="checkbox"/> Printer Cable <input checked="" type="checkbox"/> Static Bag <input type="checkbox"/> 12V DC Cable Notes: _____ _____ _____ _____ _____ _____ _____ _____ _____ _____		<input checked="" type="checkbox"/> Breath Tube Screen <input checked="" type="checkbox"/> Replace External O-Rings <input checked="" type="checkbox"/> Instrument Set Up Verified <input checked="" type="checkbox"/> R-Value <u>179</u> <input checked="" type="checkbox"/> Flow Verification (L/s) Flow Column # <u>ATP104</u> 32 mm <u>0.164</u> (.139 - .169) 36 mm <u>0.179</u> (.156 - .190) 53 mm <u>0.250</u> (.228 - .278) 103 mm <u>0.503</u> (.447 - .547) <input checked="" type="checkbox"/> Barometric Pressure Check Gauge ID # <u>26932</u> <input checked="" type="checkbox"/> Stability Checks			Flow Column # _____ <input type="checkbox"/> 5L/min - 17mm <input type="checkbox"/> 15L/min - 53mm <input type="checkbox"/> 30L/min - 103mm <input type="checkbox"/> R-Value _____ <input type="checkbox"/> Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547)																																									
		<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #/Exp</th></tr></thead><tbody><tr><td>0.050</td><td>MP5094</td><td>202201C 01/11/2024</td></tr><tr><td>0.080</td><td>MP5095</td><td>202201D 01/18/2024</td></tr><tr><td>0.200</td><td>MP5096</td><td>202201E 01/18/2024</td></tr><tr><td>0.080 DGS</td><td>N/A</td><td>AG223802 08/26/2024</td></tr></tbody></table>			Simulator	Serial #	Lot #/Exp	0.050	MP5094	202201C 01/11/2024	0.080	MP5095	202201D 01/18/2024	0.200	MP5096	202201E 01/18/2024	0.080 DGS	N/A	AG223802 08/26/2024	Maintenance By _____ <input type="checkbox"/> Battery Replacement <input type="checkbox"/> Dry Gas Regulator Replacement <input type="checkbox"/> Breath Tube Replacement <input type="checkbox"/> Other _____ _____ _____ _____ _____ _____																										
Simulator	Serial #	Lot #/Exp																																												
0.050	MP5094	202201C 01/11/2024																																												
0.080	MP5095	202201D 01/18/2024																																												
0.200	MP5096	202201E 01/18/2024																																												
0.080 DGS	N/A	AG223802 08/26/2024																																												
Calibration Adjustment By _____		Department Inspection By <u>TDG</u>																																												
Barometric Pressure Gauge _____ ID # _____		Barometric Pressure ID# <u>26932</u> Gauge <u>1016</u> Instrument <u>1015</u> Mouth Alcohol Solution Lot # <u>2021-D</u> Acetone Stock Solution Lot # <u>2022-B</u>																																												
<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.000</td><td></td><td>N/A</td><td>N/A</td></tr><tr><td>0.040</td><td></td><td></td><td></td></tr><tr><td>0.100</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.300</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table>		Simulator	Serial #	Lot #	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			<table border="1"><thead><tr><th>Simulator</th><th>Serial Number</th></tr></thead><tbody><tr><td>0.000</td><td>MP5092</td></tr><tr><td>Interferent</td><td>MP5093</td></tr><tr><td>0.050</td><td>MP5094</td></tr><tr><td>0.080</td><td>MP5095</td></tr><tr><td>0.200</td><td>MP5096</td></tr></tbody></table>					Simulator	Serial Number	0.000	MP5092	Interferent	MP5093	0.050	MP5094	0.080	MP5095	0.200	MP5096
Simulator	Serial #	Lot #	Expiration																																											
0.000		N/A	N/A																																											
0.040																																														
0.100																																														
0.200																																														
0.300																																														
0.080 DGS	N/A																																													
Simulator	Serial Number																																													
0.000	MP5092																																													
Interferent	MP5093																																													
0.050	MP5094																																													
0.080	MP5095																																													
0.200	MP5096																																													
<input type="checkbox"/> Post Calibration Adjustment Stability Checks		Attachments <input checked="" type="checkbox"/> Form 41 <input type="checkbox"/> Post-Stability Checks <input checked="" type="checkbox"/> Stability Checks <input type="checkbox"/> Flow Calibration <input checked="" type="checkbox"/> Calibration Certificate <input type="checkbox"/> Form 40 <input type="checkbox"/> Calibration Adjustment <input type="checkbox"/> Other _____																																												
<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.050</td><td></td><td></td><td></td></tr><tr><td>0.080</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table>		Simulator	Serial #	Lot #	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			<input checked="" type="checkbox"/> Instrument Complies with Chapter 11D-8, FAC <input type="checkbox"/> Instrument Does Not Comply with Chapter 11D-8, FAC <input checked="" type="checkbox"/> Return to/Place into Evidentiary Use <input type="checkbox"/> Remain Out of Evidentiary Use <input checked="" type="checkbox"/> Conduct an Agency Inspection Before Evidentiary Use																								
Simulator	Serial #	Lot #	Expiration																																											
0.050																																														
0.080																																														
0.200																																														
0.080 DGS	N/A																																													
Notes/Suggested Service: _____ _____ _____ _____ _____ _____ _____ _____ _____		Israel Soto <small>Digitally signed by Israel Soto Date: 2023.08.21 14:12:57 (+0400)</small> Phil Nicodemo <small>Digitally signed by Phil Nicodemo Date: 2023.08.25 08:11:11 -04'00'</small> Tech Review / Date _____ Admin Review / Date _____																																												

Stability Checks

0.05g/210L	0.08g/210L	0.20g/210L	DGS 0.08g/210L																																																																																																																																																
0.047 to 0.053	0.077 to 0.083	0.194 to 0.206	0.077 to 0.083																																																																																																																																																
<p>FORT LAUDERDALE PD Intoxilyzer - Alcohol Analyzer Model 8000 08/21/2023 Software: 8100.27</p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:42</td></tr> <tr><td>Control Test</td><td>0.049</td><td>09:42</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:43</td></tr> <tr><td>Control Test</td><td>0.049</td><td>09:43</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:44</td></tr> <tr><td>Control Test</td><td>0.048</td><td>09:45</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:45</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0487</td><td></td></tr> <tr><td>Std Dev</td><td>0.0006</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>1.1863</td><td></td></tr> </tbody> </table> <p>Operator's Signature </p>	Test	g/210L	Time	Air Blank	0.000	09:42	Control Test	0.049	09:42	Air Blank	0.000	09:43	Control Test	0.049	09:43	Air Blank	0.000	09:44	Control Test	0.048	09:45	Air Blank	0.000	09:45	Control Test Stats			Average	0.0487		Std Dev	0.0006		Rel Std Dev(%)	1.1863		<p>FORT LAUDERDALE PD Intoxilyzer - Alcohol Analyzer Model 8000 08/21/2023 Software: 8100.27</p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:48</td></tr> <tr><td>Control Test</td><td>0.078</td><td>09:49</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:50</td></tr> <tr><td>Control Test</td><td>0.078</td><td>09:50</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:51</td></tr> <tr><td>Control Test</td><td>0.078</td><td>09:52</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:52</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0780</td><td></td></tr> <tr><td>Std Dev</td><td>0.0000</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>0.0000</td><td></td></tr> </tbody> </table> <p>Operator's Signature </p>	Test	g/210L	Time	Air Blank	0.000	09:48	Control Test	0.078	09:49	Air Blank	0.000	09:50	Control Test	0.078	09:50	Air Blank	0.000	09:51	Control Test	0.078	09:52	Air Blank	0.000	09:52	Control Test Stats			Average	0.0780		Std Dev	0.0000		Rel Std Dev(%)	0.0000		<p>FORT LAUDERDALE PD Intoxilyzer - Alcohol Analyzer Model 8000 08/21/2023 Software: 8100.27</p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:55</td></tr> <tr><td>Control Test</td><td>0.198</td><td>09:56</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:57</td></tr> <tr><td>Control Test</td><td>0.199</td><td>09:57</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:58</td></tr> <tr><td>Control Test</td><td>0.199</td><td>09:58</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:59</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.1987</td><td></td></tr> <tr><td>Std Dev</td><td>0.0006</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>0.2906</td><td></td></tr> </tbody> </table> <p>Operator's Signature </p>	Test	g/210L	Time	Air Blank	0.000	09:55	Control Test	0.198	09:56	Air Blank	0.000	09:57	Control Test	0.199	09:57	Air Blank	0.000	09:58	Control Test	0.199	09:58	Air Blank	0.000	09:59	Control Test Stats			Average	0.1987		Std Dev	0.0006		Rel Std Dev(%)	0.2906		<p>  FORT LAUDERDALE PD Intoxilyzer - Alcohol Analyzer Model 8000 08/21/2023 Software: 8100.27 </p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:37</td></tr> <tr><td>Control Test</td><td>0.080</td><td>09:37</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:37</td></tr> <tr><td>Control Test</td><td>0.079</td><td>09:38</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:38</td></tr> <tr><td>Control Test</td><td>0.079</td><td>09:39</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:39</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0793</td><td></td></tr> <tr><td>Std Dev</td><td>0.0006</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>0.7277</td><td></td></tr> </tbody> </table> <p>Operator's Signature </p>	Test	g/210L	Time	Air Blank	0.000	09:37	Control Test	0.080	09:37	Air Blank	0.000	09:37	Control Test	0.079	09:38	Air Blank	0.000	09:38	Control Test	0.079	09:39	Air Blank	0.000	09:39	Control Test Stats			Average	0.0793		Std Dev	0.0006		Rel Std Dev(%)	0.7277	
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	09:42																																																																																																																																																	
Control Test	0.049	09:42																																																																																																																																																	
Air Blank	0.000	09:43																																																																																																																																																	
Control Test	0.049	09:43																																																																																																																																																	
Air Blank	0.000	09:44																																																																																																																																																	
Control Test	0.048	09:45																																																																																																																																																	
Air Blank	0.000	09:45																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0487																																																																																																																																																		
Std Dev	0.0006																																																																																																																																																		
Rel Std Dev(%)	1.1863																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	09:48																																																																																																																																																	
Control Test	0.078	09:49																																																																																																																																																	
Air Blank	0.000	09:50																																																																																																																																																	
Control Test	0.078	09:50																																																																																																																																																	
Air Blank	0.000	09:51																																																																																																																																																	
Control Test	0.078	09:52																																																																																																																																																	
Air Blank	0.000	09:52																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0780																																																																																																																																																		
Std Dev	0.0000																																																																																																																																																		
Rel Std Dev(%)	0.0000																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	09:55																																																																																																																																																	
Control Test	0.198	09:56																																																																																																																																																	
Air Blank	0.000	09:57																																																																																																																																																	
Control Test	0.199	09:57																																																																																																																																																	
Air Blank	0.000	09:58																																																																																																																																																	
Control Test	0.199	09:58																																																																																																																																																	
Air Blank	0.000	09:59																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.1987																																																																																																																																																		
Std Dev	0.0006																																																																																																																																																		
Rel Std Dev(%)	0.2906																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	09:37																																																																																																																																																	
Control Test	0.080	09:37																																																																																																																																																	
Air Blank	0.000	09:37																																																																																																																																																	
Control Test	0.079	09:38																																																																																																																																																	
Air Blank	0.000	09:38																																																																																																																																																	
Control Test	0.079	09:39																																																																																																																																																	
Air Blank	0.000	09:39																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0793																																																																																																																																																		
Std Dev	0.0006																																																																																																																																																		
Rel Std Dev(%)	0.7277																																																																																																																																																		

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: FORT LAUDERDALE PD
Time of Inspection: 11:59

Date of Inspection: 08/21/2023

Serial Number: 80-007009
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202201C Exp: 01/11/2024	0.08g/210L Test (g/210L) Lot#:202201D Exp: 01/18/2024	0.20g/210L Test (g/210L) Lot#:202201E Exp: 01/18/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG223802 Exp: 08/26/2024
0.000	0.049	0.078	0.200	0.079
0.000	0.048	0.078	0.200	0.079
0.000	0.048	0.078	0.200	0.078
0.000	0.048	0.079	0.200	0.079
0.000	0.049	0.078	0.200	0.079
0.000	0.049	0.079	0.200	0.078
0.000	0.049	0.079	0.200	0.078
0.000	0.049	0.079	0.200	0.078
0.000	0.049	0.078	0.200	0.078
0.000	0.049	0.078	0.201	0.078


Standard Deviations	0.0004	0.0005	0.0003	0.0005
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0004 Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.


I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



TAYLOR D GUTSCHOW

Signature and Printed Name

08/21/2023
Date



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
4700 Terminal Drive, Suite 1
Ft. Myers, FL 33907

This is to certify the calibration of Intoxilyzer 8000 serial number 80-007009, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-007009</u>	UNCERTAINTY* \pm
Owning Agency:	<u>FORT LAUDERDALE PD</u>	0.050 g/ 210 L 0.004
Calibration Date:	<u>08/21/2023</u>	0.080 g/ 210 L 0.004
Calibration Time:	<u>11:59</u>	0.200 g/ 210 L 0.007
		0.080 g/ 210 L Dry Gas Control 0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.

*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ($k=3$).


The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards. This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

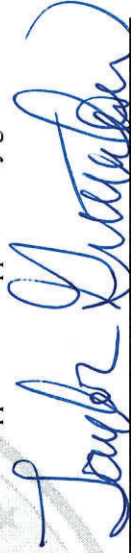

08/21/2023

Date

TAYLOR D GUTSCHOW,

Department Inspector

FDLE/ATP Form 69 December 2021

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
4700 Terminal Drive, Suite 1
Ft. Myers, FL 33907

This is to certify the calibration of Intoxilyzer 8000 serial number 80-007009, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-007009</u>	UNCERTAINTY* \pm	
Owning Agency:	<u>FT. LAUDERDALE PD</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>01/10/2023</u>	0.080 g/ 210 L	0.004
Calibration Time:	<u>10:08</u>	0.200 g/ 210 L	0.007
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.

*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ($k=3$).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.


Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards.

This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

01/10/2023

Date


DAVID E REYES-RIVERA,
Department Inspector

FDLE/ATP Form 69 December 2021

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality

Page 1 of 1

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: FT. LAUDERDALE PD
Time of Inspection: 10:08

Date of Inspection: 01/10/2023

Serial Number: 80-007009
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202201C Exp: 01/11/2024	0.08g/210L Test (g/210L) Lot#:00521080A2 Exp: 02/05/2023	0.20g/210L Test (g/210L) Lot#:202201E Exp: 01/18/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:00521080A2 Exp: 02/05/2023
0.000	0.049	0.000 / 0.079	0.200	0.081
0.000	0.049	0.000 / 0.078	0.200	0.081
0.000	0.049	0.000 / 0.079	0.200	0.080
0.000	0.049	0.000 / 0.078	0.200	0.081
0.000	0.049	0.000 / 0.078	0.200	0.081
0.000	0.050	0.000 / 0.078	0.200	0.080
0.000	0.049	0.000 / 0.079	0.200	0.081
0.000	0.050	0.000 / 0.079	0.200	0.080
0.000	0.050	0.000 / 0.078	0.200	0.081
0.000	0.050	0.000 / 0.079	0.200	0.080

Standard Deviations	0.0005	0.0000 / 0.0005	0.0000	0.0005
---------------------	--------	-----------------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5

Remarks:

08: Control Outside Tolerance USED DRY GAS.





The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 _____
Signature and Printed Name

01/10/2023
Date

Type of Test	Serial Number	Agency	Date	Performed By
Stabilities	80-007009	Ft. Lauderdale Police Department	01/10/2023	DERR <i>[Signature]</i>

0.05g/210L 0.047 to 0.053 <input checked="" type="checkbox"/>	0.08g/210L 0.077 to 0.083 <input checked="" type="checkbox"/>	0.20g/210L 0.194 to 0.206 <input checked="" type="checkbox"/>	DGS 0.08g/210L 0.077 to 0.083 <input checked="" type="checkbox"/>																																																																																																																																																									
FT. LAUDERDALE PD Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-007009 01/10/2023 Software: 8100.27	FT. LAUDERDALE PD Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-007009 01/10/2023 Software: 8100.27	FT. LAUDERDALE PD Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-007009 01/10/2023 Software: 8100.27	FT. LAUDERDALE PD Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-007009 01/10/2023 Software: 8100.27																																																																																																																																																									
<table><tr><th>Test</th><th>g/210L</th><th>Time</th></tr><tr><td>Air Blank</td><td>0.000</td><td>07:30</td></tr><tr><td>Control Test</td><td>0.049</td><td>07:30</td></tr><tr><td>Air Blank</td><td>0.000</td><td>07:31</td></tr><tr><td>Control Test</td><td>0.046</td><td>07:32</td></tr><tr><td>Air Blank</td><td>0.000</td><td>07:32</td></tr><tr><td>Control Test</td><td>0.042</td><td>07:33</td></tr><tr><td>Air Blank</td><td>0.000</td><td>07:33</td></tr><tr><td>Control Test</td><td>0.040</td><td>07:33</td></tr><tr><td>Average</td><td>0.0450</td><td></td></tr><tr><td>Std Dev</td><td>0.0000</td><td></td></tr><tr><td>Rel Std Dev(%)</td><td>0.0000</td><td></td></tr></table> <div> Operator's Signature</div>	Test	g/210L	Time	Air Blank	0.000	07:30	Control Test	0.049	07:30	Air Blank	0.000	07:31	Control Test	0.046	07:32	Air Blank	0.000	07:32	Control Test	0.042	07:33	Air Blank	0.000	07:33	Control Test	0.040	07:33	Average	0.0450		Std Dev	0.0000		Rel Std Dev(%)	0.0000		<table><tr><th>Test</th><th>g/210L</th><th>Time</th></tr><tr><td>Air Blank</td><td>0.078</td><td>07:35</td></tr><tr><td>Control Test</td><td>0.078</td><td>07:36</td></tr><tr><td>Air Blank</td><td>0.076</td><td>07:37</td></tr><tr><td>Control Test</td><td>0.075</td><td>07:37</td></tr><tr><td>Air Blank</td><td>0.077</td><td>07:38</td></tr><tr><td>Control Test</td><td>0.075</td><td>07:38</td></tr><tr><td>Air Blank</td><td>0.080</td><td>07:39</td></tr><tr><td>Control Test</td><td>0.080</td><td>07:39</td></tr><tr><td>Control Test Stats</td><td></td><td></td></tr><tr><td>Average</td><td>0.0787</td><td></td></tr><tr><td>Std Dev</td><td>0.0000</td><td></td></tr><tr><td>Rel Std Dev(%)</td><td>0.7359</td><td></td></tr></table> <div> Operator's Signature</div>	Test	g/210L	Time	Air Blank	0.078	07:35	Control Test	0.078	07:36	Air Blank	0.076	07:37	Control Test	0.075	07:37	Air Blank	0.077	07:38	Control Test	0.075	07:38	Air Blank	0.080	07:39	Control Test	0.080	07:39	Control Test Stats			Average	0.0787		Std Dev	0.0000		Rel Std Dev(%)	0.7359		<table><tr><th>Test</th><th>g/210L</th><th>Time</th></tr><tr><td>Air Blank</td><td>0.000</td><td>07:41</td></tr><tr><td>Control Test</td><td>0.200</td><td>07:42</td></tr><tr><td>Air Blank</td><td>0.000</td><td>07:42</td></tr><tr><td>Control Test</td><td>0.199</td><td>07:43</td></tr><tr><td>Air Blank</td><td>0.000</td><td>07:44</td></tr><tr><td>Control Test</td><td>0.200</td><td>07:44</td></tr><tr><td>Air Blank</td><td>0.000</td><td>07:45</td></tr><tr><td>Control Test</td><td>0.200</td><td>07:45</td></tr><tr><td>Control Test Stats</td><td></td><td></td></tr><tr><td>Average</td><td>0.1997</td><td></td></tr><tr><td>Std Dev</td><td>0.0000</td><td></td></tr><tr><td>Rel Std Dev(%)</td><td>0.2892</td><td></td></tr></table> <div> Operator's Signature</div>	Test	g/210L	Time	Air Blank	0.000	07:41	Control Test	0.200	07:42	Air Blank	0.000	07:42	Control Test	0.199	07:43	Air Blank	0.000	07:44	Control Test	0.200	07:44	Air Blank	0.000	07:45	Control Test	0.200	07:45	Control Test Stats			Average	0.1997		Std Dev	0.0000		Rel Std Dev(%)	0.2892		<table><tr><th>Test</th><th>g/210L</th><th>Time</th></tr><tr><td>Air Blank</td><td>0.000</td><td>07:46</td></tr><tr><td>Control Test</td><td>0.080</td><td>07:46</td></tr><tr><td>Air Blank</td><td>0.000</td><td>07:46</td></tr><tr><td>Control Test</td><td>0.081</td><td>07:47</td></tr><tr><td>Air Blank</td><td>0.000</td><td>07:47</td></tr><tr><td>Control Test</td><td>0.081</td><td>07:48</td></tr><tr><td>Air Blank</td><td>0.000</td><td>07:48</td></tr><tr><td>Control Test</td><td>0.080</td><td>07:49</td></tr><tr><td>Control Test Stats</td><td></td><td></td></tr><tr><td>Average</td><td>0.0807</td><td></td></tr><tr><td>Std Dev</td><td>0.0000</td><td></td></tr><tr><td>Rel Std Dev(%)</td><td>0.7157</td><td></td></tr></table> <div> Operator's Signature</div>	Test	g/210L	Time	Air Blank	0.000	07:46	Control Test	0.080	07:46	Air Blank	0.000	07:46	Control Test	0.081	07:47	Air Blank	0.000	07:47	Control Test	0.081	07:48	Air Blank	0.000	07:48	Control Test	0.080	07:49	Control Test Stats			Average	0.0807		Std Dev	0.0000		Rel Std Dev(%)	0.7157	
Test	g/210L	Time																																																																																																																																																										
Air Blank	0.000	07:30																																																																																																																																																										
Control Test	0.049	07:30																																																																																																																																																										
Air Blank	0.000	07:31																																																																																																																																																										
Control Test	0.046	07:32																																																																																																																																																										
Air Blank	0.000	07:32																																																																																																																																																										
Control Test	0.042	07:33																																																																																																																																																										
Air Blank	0.000	07:33																																																																																																																																																										
Control Test	0.040	07:33																																																																																																																																																										
Average	0.0450																																																																																																																																																											
Std Dev	0.0000																																																																																																																																																											
Rel Std Dev(%)	0.0000																																																																																																																																																											
Test	g/210L	Time																																																																																																																																																										
Air Blank	0.078	07:35																																																																																																																																																										
Control Test	0.078	07:36																																																																																																																																																										
Air Blank	0.076	07:37																																																																																																																																																										
Control Test	0.075	07:37																																																																																																																																																										
Air Blank	0.077	07:38																																																																																																																																																										
Control Test	0.075	07:38																																																																																																																																																										
Air Blank	0.080	07:39																																																																																																																																																										
Control Test	0.080	07:39																																																																																																																																																										
Control Test Stats																																																																																																																																																												
Average	0.0787																																																																																																																																																											
Std Dev	0.0000																																																																																																																																																											
Rel Std Dev(%)	0.7359																																																																																																																																																											
Test	g/210L	Time																																																																																																																																																										
Air Blank	0.000	07:41																																																																																																																																																										
Control Test	0.200	07:42																																																																																																																																																										
Air Blank	0.000	07:42																																																																																																																																																										
Control Test	0.199	07:43																																																																																																																																																										
Air Blank	0.000	07:44																																																																																																																																																										
Control Test	0.200	07:44																																																																																																																																																										
Air Blank	0.000	07:45																																																																																																																																																										
Control Test	0.200	07:45																																																																																																																																																										
Control Test Stats																																																																																																																																																												
Average	0.1997																																																																																																																																																											
Std Dev	0.0000																																																																																																																																																											
Rel Std Dev(%)	0.2892																																																																																																																																																											
Test	g/210L	Time																																																																																																																																																										
Air Blank	0.000	07:46																																																																																																																																																										
Control Test	0.080	07:46																																																																																																																																																										
Air Blank	0.000	07:46																																																																																																																																																										
Control Test	0.081	07:47																																																																																																																																																										
Air Blank	0.000	07:47																																																																																																																																																										
Control Test	0.081	07:48																																																																																																																																																										
Air Blank	0.000	07:48																																																																																																																																																										
Control Test	0.080	07:49																																																																																																																																																										
Control Test Stats																																																																																																																																																												
Average	0.0807																																																																																																																																																											
Std Dev	0.0000																																																																																																																																																											
Rel Std Dev(%)	0.7157																																																																																																																																																											