

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: NAS JACKSONVILLE PD
Time of Inspection: 12:14

Date of Inspection: 01/31/2024

Serial Number: 80-000778
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#: 202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#: 202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 08223090A3 Exp: 06/05/2025
0.000	0.050	0.079	0.199	0.082
0.000	0.050	0.079	0.200	0.082
0.000	0.050	0.080	0.201	0.082

Number of Simulators Used: 5


Remarks:

Amended inspection: Per FDLE/ATP, Instrument removed from service @NAS Jax due to inability to connect to server to upload. Sent to FDLE/ATP for upload and yearly Departmental Inspection.
Sgt. M Potter 7599

 7599

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

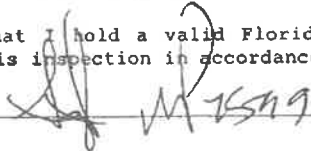

MICHAEL R. POTTER
Signature and Printed Name

01/31/2024
Date