

Florida Department of Law Enforcement

Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: HAMILTON COUNTY SO
Time of Inspection: 00:51

Date of Inspection: 11/26/2024

Serial Number: 80-000797
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: A-200	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#: 202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#: 202307C Exp: 07/12/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 10124080A2 Exp: 06/05/2026
0.000	0.048	0.076	0.190	0.083
0.000	0.048	0.077	0.192	0.082
0.000	0.048	0.077	0.193	0.082

Number of Simulators Used: 4

Remarks:

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

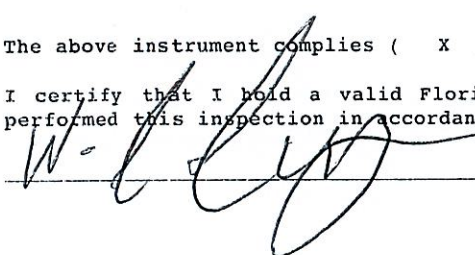

WILLIAM C CURRY

Signature and Printed Name

11/26/2024
Date