

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: PORT RICHEY PD
Time of Inspection: 08:45

Date of Inspection: 09/30/2024

Serial Number: 80-000967
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#: 202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#: 202307C Exp: 07/12/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 402816921 Exp: 08/09/2026
0.000	0.048	0.077	0.192	0.078
0.000	0.048	0.078	0.194	0.078
0.000	0.048	0.078	0.195	0.078

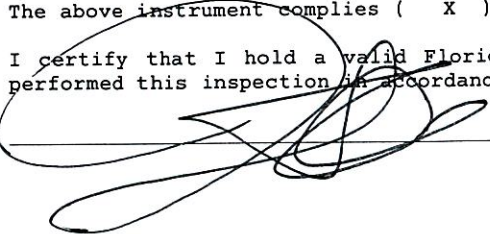
Number of Simulators Used: 5

Remarks: While Attempting to upload Received ERROR 012 Disabled Mode
INSTRUMENT SENT TO FDLE TO CLEAR THE ERROR —

ofc. J. McCONNELL 909
PRG15 AI

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


Signature and Printed Name

JEFFREY W MCCONNELL

09/30/2024
Date