

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD
Time of Inspection: 09:18

Date of Inspection: 06/11/2024

Serial Number: 80-000996
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#:202307C Exp: 07/12/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:28423080A3 Exp: 11/05/2025
0.000	0.047	0.076	0.189 / 0.195	0.085
0.000	0.048	0.077	0.196 / 0.196	0.085
0.000	0.048	0.078	0.196 / 0.195	0.085


Number of Simulators Used: 5

Remarks:

20: Control Outside Tolerance CHECKED SEAL.

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

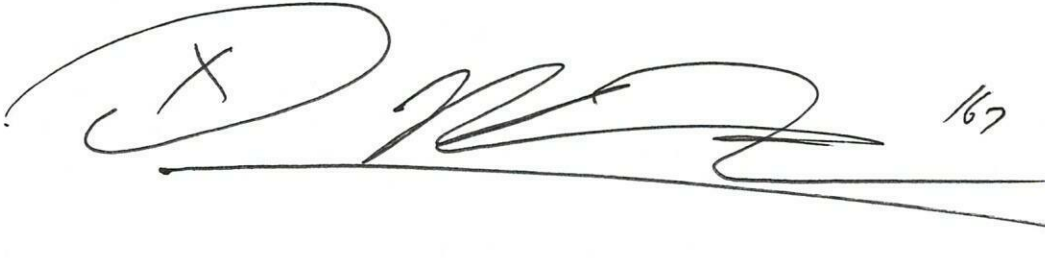

 MATTHEW S RASMUSSEN
 Signature and Printed Name

06/11/2024
 Date

TITUSVILLE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000996
06/11/2024
Software: 8100.27

DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

 167

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD
Time of Inspection: 09:02

Date of Inspection: 05/21/2024

Serial Number: 80-000996
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#:202307C Exp: 07/12/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:28423080A3 Exp: 11/05/2025
0.000	0.046	0.077	0.193	0.084
0.000	0.047	0.078	0.196	0.084
0.000	0.047	0.078	0.196	0.084

Number of Simulators Used: 5

Remarks:
N/A

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MATTHEW S RASMUSSEN

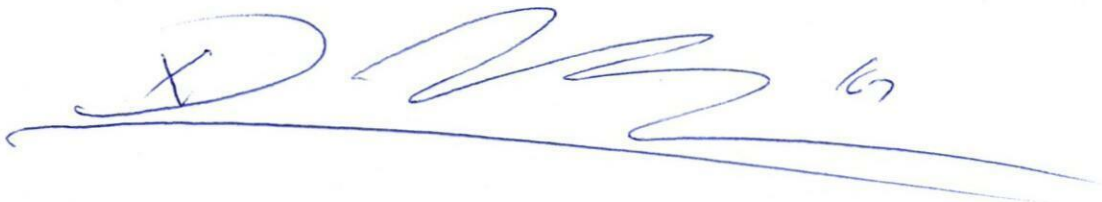
Signature and Printed Name

05/21/2024
Date

TITUSVILLE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000996
05/21/2024
Software: 8100.27

DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

 67

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD
Time of Inspection: 15:59

Date of Inspection: 04/22/2024

Serial Number: 80-000996
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted	Yes	
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#:202307C Exp: 07/12/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:28423080A3 Exp: 11/15/2025
0.000	0.047	0.076	0.191	0.087 / 0.084
0.000	0.047	0.077	0.193	0.087 / 0.084
0.000	0.047	0.077	0.193	0.087 / 0.084

Number of Simulators Used: 5

Remarks:

Time-Date changed. 08: Control Outside Tolerance.

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MATTHEW S RASMUSSEN

Signature and Printed Name

04/22/2024
Date

TITUSVILLE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000996
04/22/2024
Software: 8100.27

DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

A large, stylized handwritten signature in black ink, spanning across the lower half of the page. The signature is fluid and cursive, with a long horizontal stroke at the end. To the right of the main signature, there is a small handwritten mark that appears to be "187".

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD

Time of Inspection: 12:19

Date of Inspection: 02/05/2024

Serial Number: 80-000996

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#:202307C Exp: 07/12/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:231592 Exp: 11/15/2025
0.000	0.048	0.078	0.193	0.084
0.000	0.048	0.077	0.197	0.084
0.000	0.048	0.077	0.196	0.084

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

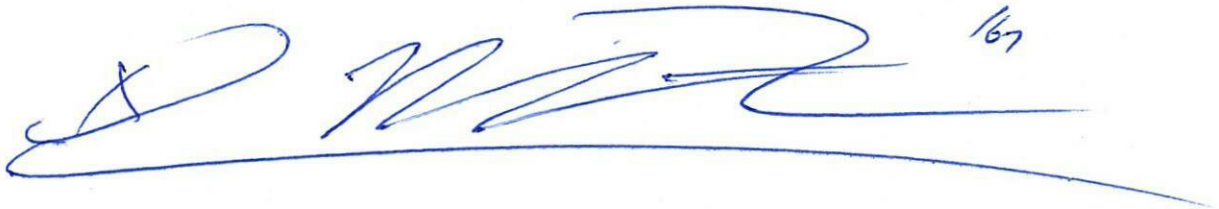
 MATTHEW S RASMUSSEN
Signature and Printed Name

02/05/2024
Date

TITUSVILLE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000996
02/05/2024
Software: 8100.27

DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

 167