

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD
Time of Inspection: 10:23

Date of Inspection: 12/30/2024

Serial Number: 80-001649
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:
0.000	INT / 0.045			
0.000	/ 0.044			
0.000	/ 0.043			

Number of Simulators Used: 5

Remarks:

05: Interferent Detect CHANGED INPUT HOSE , Control Outside. INT DETECT CHANGED INPUT HOSE Non-compliance:LOW RANGE ON 0.05 ARS.

*checked Seal on Sim used And HOSE
ReAct of Agency Inspection*

The above instrument complies () does not comply (☒) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 167 MATTHEW S RASMUSSEN
Signature and Printed Name

12/30/2024
Date

TITUSVILLE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001649
12/30/2024
Software: 8100.27

DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

(X)  107

TITUSVILLE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001649
12/30/2024
Software: 8100.27

DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

A handwritten signature consisting of a large 'X' inside a circle, followed by a stylized signature, and the number '167' to the right. A long horizontal line is drawn underneath the signature.

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD
Time of Inspection: 12:11

Date of Inspection: 12/30/2024

Serial Number: 80-001649
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202410E Exp: 10/22/2026	0.20g/210L Test (g/210L) Lot#:202307C Exp: 07/12/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:231592 Exp: 11/15/2025
0.000	0.047	0.078	0.196	0.081
0.000	0.048	0.078	0.194	0.081
0.000	0.048	0.079	0.198	0.081

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MATTHEW S RASMUSSEN

Signature and Printed Name

12/30/2024
Date

TITUSVILLE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001649
12/30/2024
Software: 8100.27

DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

A handwritten signature in dark ink, consisting of a stylized 'X' inside a circle followed by a series of loops and a long horizontal stroke. To the right of the signature, the date '1/2' is written.

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD

Time of Inspection: 21:12

Date of Inspection: 10/29/2024

Serial Number: 80-001649

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#:202307C Exp: 07/12/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:231592 Exp: 11/05/2025
0.000	0.046	0.077	0.191	0.082
0.000	0.047	0.077	0.195	0.081
0.000	0.047	0.077	0.196	0.082

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MATTHEW S RASMUSSEN

Signature and Printed Name

10/29/2024
Date

TITUSVILLE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001649
10/29/2024
Software: 8100.27

DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

 167

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD
Time of Inspection: 13:56

Date of Inspection: 09/17/2024

Serial Number: 80-001649
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#:202307C Exp: 07/12/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:231592 Exp: 11/05/2025
0.000	0.046	0.077	0.195	0.081
0.000	0.046	0.076	0.195	0.081
0.000	0.047	0.076	0.196	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


MATTHEW S RASMUSSEN

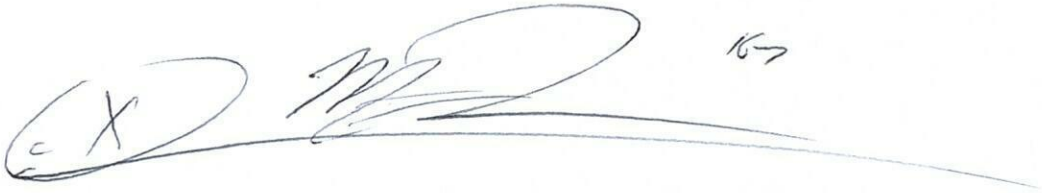
Signature and Printed Name

09/17/2024
Date

TITUSVILLE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001649
09/17/2024
Software: 8100.27

DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

A large, stylized handwritten signature in blue ink, starting with a large 'X' inside a circle, followed by a long horizontal stroke. To the right of the signature is a small handwritten mark that looks like '167'.

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD

Time of Inspection: 17:06

Date of Inspection: 07/02/2024

Serial Number: 80-001649

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#:202307C Exp: 07/12/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:231592 Exp: 11/05/2025
0.000	0.044 / 0.045	0.075	0.189 / 0.194	0.081
0.000	0.045 / 0.045	0.076	0.190 / 0.195	0.081
0.000	0.045 / 0.046	0.076	0.190 / 0.196	0.081

Number of Simulators Used: 5

Remarks:

05: Control Outside Tolerance CHECKED SEAL. 20: Control Outside Tolerance CHECKED SEAL AND VENT OF R OOM.

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 167

Signature and Printed Name

MATTHEW S RASMUSSEN

07/02/2024
Date

TITUSVILLE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001649
07/02/2024
Software: 8100.27

DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

(X)  167

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD

Time of Inspection: 10:52

Date of Inspection: 06/11/2024

Serial Number: 80-001649

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#:202307C Exp: 07/12/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:231592 Exp: 11/05/2025
0.008 / 0.000	0.040 / 0.047	0.076	0.190	0.080
0.000 / 0.000	0.045 / 0.048	0.077	0.196	0.081
0.000 / 0.000	0.048 / 0.049	0.078	0.196	0.081

Number of Simulators Used: 5

Remarks:

00: Control Outside Tolerance RESIDUAL SOLUTION IN TUBE. 05: Control Outside Tolerance CHECKED SEAL.

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

MATTHEW S RASMUSSEN

Signature and Printed Name

06/11/2024
Date

TITUSVILLE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001649
06/11/2024
Software: 8100.27

DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

 167