

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: ALACHUA PD

Time of Inspection: 23:16

Date of Inspection: 07/10/2024

Serial Number: 80-001720

Software: 8100.27

| Check or Test                               | YES | NO |
|---------------------------------------------|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |


|                            |                                                             |                                                             |                                                             |                                                                             |
|----------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-------------------------------------------------------------|-----------------------------------------------------------------------------|
| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202303J<br>Exp: 03/28/2025 | 0.08g/210L Test (g/210L)<br>Lot#:202307A<br>Exp: 07/11/2025 | 0.20g/210L Test (g/210L)<br>Lot#:202307C<br>Exp: 07/12/2025 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:26422080A1<br>Exp: 11/05/2024 |
| 0.000                      | 0.049                                                       | 0.080                                                       | 0.199                                                       | 0.079                                                                       |
| 0.000                      | 0.050                                                       | 0.081                                                       | 0.200                                                       | 0.080                                                                       |
| 0.000                      | 0.050                                                       | 0.081                                                       | 0.200                                                       | 0.080                                                                       |

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

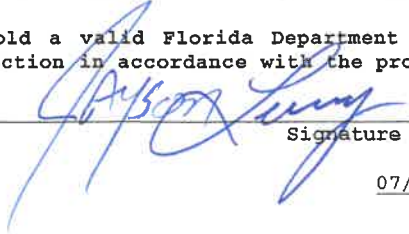

JAYSON I LEVY

Signature and Printed Name

07/10/2024  
Date