

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 09:21

Date of Inspection: 05/21/2024

Serial Number: 80-006472
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

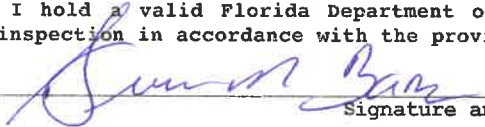
Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402357111 Exp: 02/10/2025
0.000	0.048	0.078	0.197	0.081
0.000	0.049	0.078	0.198	0.080
0.000	0.049	0.079	0.198	0.080

Number of Simulators Used: 5

Remarks:
NA

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


 SUSAN M BARGE
 Signature and Printed Name

05/21/2024
Date

Florida Department of Law Enforcement

Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 13:19

Date of Inspection: 03/22/2024

Serial Number: 80-006472
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

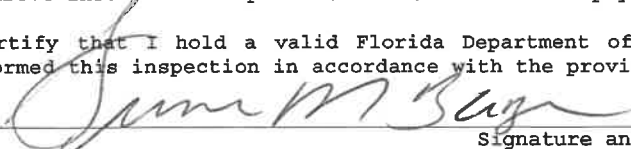
Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402357111 Exp: 02/10/2025
0.000	0.045	0.075	0.191	0.080
0.000	0.046	0.076	0.192	0.080
0.000	0.046	0.076	0.193	0.079

Number of Simulators Used: 5

Remarks:
N

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


Signature and Printed Name SUSAN M 5

03/22/2024
Date