

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: BROWARD COUNTY SO
Time of Inspection: 11:51

Date of Inspection: 08/07/2024

Serial Number: 80-006475
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#:202307C Exp: 07/12/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402783528 Exp: 06/27/2026
0.000	0.048	0.078	0.198	0.071 / 0.000
0.000	0.048	0.078	0.198	0.000 / 0.078
0.000	0.048	0.078	0.198	0.000 / 0.078

Number of Simulators Used: 5

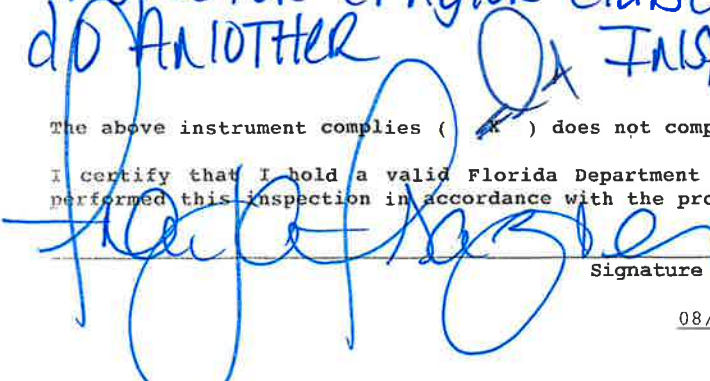
Remarks:

08: Control Outside Tolerance, DRY GAS LOOSE.

The Dry Gas was loose
I realized the tank was loose after the first analysis on the second test. The instrument was not in compliance as a result of the dry gas being loose. Spoke with the department inspector (Taylor Gutschow) He advised me to do another inspection.

The above instrument complies (☒) does not comply (☒) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


Signature and Printed Name

ANAYA S. FRAZIER

08/07/2024
Date