

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO
Time of Inspection: 14:21

Date of Inspection: 02/12/2024

Serial Number: 80-006559
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202307A Exp: 07/11/2025	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402558895 Exp: 10/03/2025
0.000	0.049	0.079	0.198	0.082
0.000	0.049	0.079	0.198	0.082
0.000	0.049	0.079	0.198	0.081

Number of Simulators Used: 5

Remarks:


HAD TO RE-DO TEST ^V TO POWER OUTAGE

Due

WDC

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

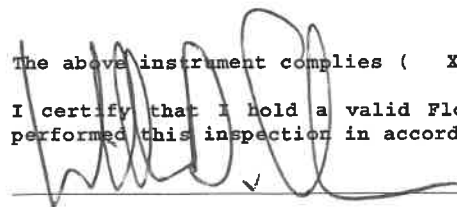

WILLIAM COLEMAN

Signature and Printed Name

02/12/2024
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO
Time of Inspection: 13:22

Date of Inspection: 02/12/2024

Serial Number: 80-006559
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08g/210L Test (g/210L) Lot#:_____ Exp:_____	0.20g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:_____ Exp:_____
0.000				
0.000				
0.000				

Number of Simulators Used: 5


Remarks:

Int Det: INT NOT CONNECTED, RFI Detect. Non-compliance: X

Interferent was disconnected. Re-connected. During iteration 3 we received an RFI detect. Located the RFI source and ~~re~~ connected & conducted another round of inspection.

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

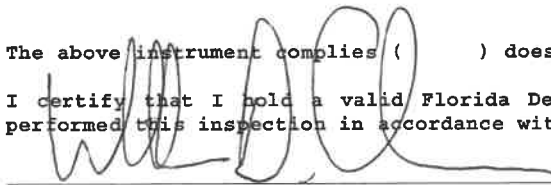

WILLIAM COLEMAN

Signature and Printed Name

02/12/2024
Date