

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: Broward County SO
Time of Inspection:

Serial Number: 80-006924
Date of Inspection: June 2024

Software: 8100.27

CHECK OR TEST	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		
Alcohol Free Subject Test: 0.000		
Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect		
Diagnostic Check (Post-Inspection): OK		


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Number of Simulators Used: _____

Remarks: Inspection was not conducted as the instrument was sent to CMI, Inc for repairs.

The above instrument complies (____) does not comply (____) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

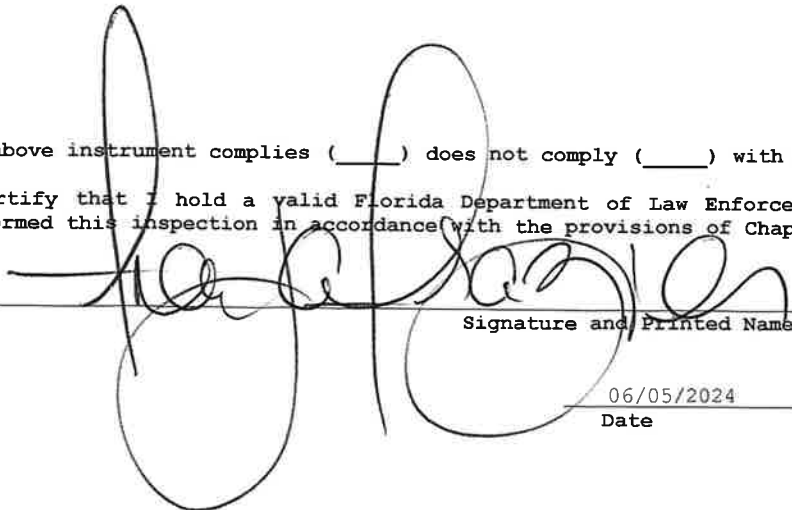

Anaya Frazier

Signature and Printed Name

06/05/2024
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: Broward County SO

Serial Number: 80-006924

Time of Inspection:

Date of Inspection: May 2024

Software: 8100.27

CHECK OR TEST	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		
Alcohol Free Subject Test: 0.000		
Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect		
Diagnostic Check (Post-Inspection): OK		


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Number of Simulators Used: _____

Remarks: Inspection was not conducted as the instrument was sent to CMI, Inc for repairs.

The above instrument complies (____) does not comply (____) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

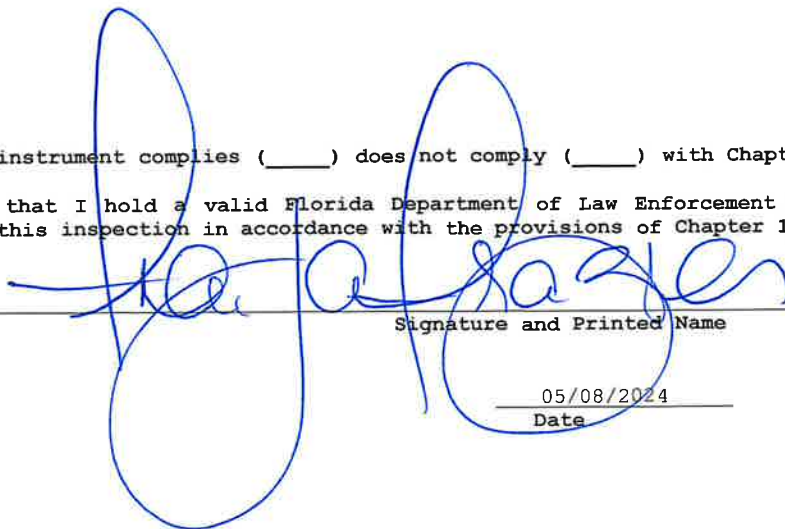

Anaya Frazier

Signature and Printed Name

05/08/2024

Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: Broward County SO

Serial Number: 80-006924

Time of Inspection:

Date of Inspection: April 2024

Software: 8100.27

CHECK OR TEST	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		
Alcohol Free Subject Test: 0.000		
Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect		
Diagnostic Check (Post-Inspection): OK		

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Number of Simulators Used: _____

Remarks: Inspection was not conducted as the instrument was sent to CMI, Inc for repairs.

The above instrument complies (____) does not comply (____) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Anaya Frazier

Signature and Printed Name

04/10/2024

Date