



Florida Department of
Law Enforcement

AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Miami PD

Instrument Serial Number: 80-007516

AGENCY INSPECTION DISCREPENCY

Agency Inspector: Angel Fernandez

Inspection Date: 01/22/2024

☐ A test was repeated without reason for repeat or the corrective action given

☐ Alcohol Free/Mouth Alcohol ☐ Alcohol Free Test ☐ Interferent Detect

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Agency Inspection not conducted for calendar month

☒ Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☒ 0.080 g/210L Dry Gas

☐ Lot Number and/or Expiration Date for Standards entered incorrectly

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Other Electronic Data Review/Comments:

REQUESTED CORRECTIVE ACTION

☒ Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector

☐ Provide written explanation regarding referenced item(s) to Department Inspector

☐ Remove instrument from evidentiary use until otherwise directed by the Department

☐ Other:

Taylor Gutschow

Digitally signed by Taylor

Gutschow

Date: 2024.02.14 11:41:34 -05'00'

02/14/2024

Signature of Alcohol Testing Program Staff Member

Date

Florida Department of Law Enforcement

AMENDED Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MIAMI PD
Time of Inspection: 13:34

Date of Inspection: 01/22/2024

Serial Number: 80-007516
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1506449 ²⁰²⁴ Exp: 06/10/2023 <i>AF 28394</i>
0.000	0.049	0.077	0.200	0.081
0.000	0.049	0.078	0.200	0.080
0.000	0.049	0.077	0.200	0.081

Number of Simulators Used: 5

Remarks:


AMENDED DRY GAS EXPIRATION YEAR. CLERICAL ERROR.



28394 2/21/2024

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

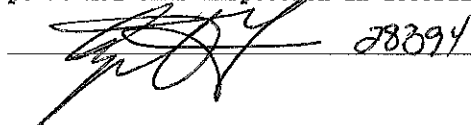

ANGEL FERNANDEZ
Signature and Printed Name

01/22/2024
Date