



INSTRUMENT PROCESSING SHEET

Agency Okaloosa County SOS/N 80-00763 000763 DA 12/16/24Florida Department of
Law EnforcementDate In 11/26/2024 DI Completion Date 12/10/2024☐ Ship ☒ P/U ☐ H/D ☐ CMI ☐ EE

Intake	By <u>ALL</u>	Date <u>12/02/2024</u>	Quality Checks	By <u>DA</u>	Date <u>12/05/2024</u>	Flow Calibration	By _____	Date _____																												
☒ Annual ☐ Registration ☐ Return from CMI / EE Visual Inspection: ☒ Case ☒ Handle ☒ Keyboard ☒ Dry Gas Shelf ☒ Feet ☒ Breath Tube ☒ Ports ☒ Screws Tight Other Equipment/ Accessories: ☐ Power cord ☐ Printer Cable ☐ Static Bag ☐ 12V DC Cable Notes: <u>dropoff, no box</u>			☒ Breath Tube Screen ☒ Replace External O-Rings ☒ Instrument Set Up Verified ☒ R-Value <u>201</u> ☒ Flow Verification (L/s) Flow Column # <u>ATP103</u> 32 mm <u>0.144</u> (.139 - .169) 36 mm <u>0.156</u> (.156 - .190) 53 mm <u>0.234</u> (.228 - .278) 103 mm <u>0.511</u> (.447 - .547) ☒ Barometric Pressure Check Gauge ID # <u>30793</u> ☒ Stability Checks			Flow Column # _____ ☐ 5L/min – 17mm ☐ 15L/min – 53mm ☐ 30L/min – 103mm ☐ R-Value _____ ☐ Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547)																														
			<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #/Exp</th></tr></thead><tbody><tr><td>0.050</td><td>MP6291</td><td>202406K 06/19/2026</td></tr><tr><td>0.080</td><td>MP6292</td><td>202406L 06/19/2026</td></tr><tr><td>0.200</td><td>MP6293</td><td>202406N 06/20/2026</td></tr><tr><td>0.080 DGS</td><td>N/A</td><td>AG325603 09/13/2025</td></tr></tbody></table>	Simulator	Serial #	Lot #/Exp	0.050	MP6291	202406K 06/19/2026	0.080	MP6292	202406L 06/19/2026	0.200	MP6293	202406N 06/20/2026	0.080 DGS	N/A	AG325603 09/13/2025			<table border="1"><thead><tr><th colspan="2">Maintenance By <u>DA</u> Date <u>12/5/24</u></th></tr></thead><tbody><tr><td>☐ Battery Replacement</td><td></td></tr><tr><td>☒ Dry Gas Regulator Replacement</td><td></td></tr><tr><td>☐ Breath Tube Replacement</td><td></td></tr><tr><td>☐ Other _____</td><td></td></tr></tbody></table>	Maintenance By <u>DA</u> Date <u>12/5/24</u>		☐ Battery Replacement		☒ Dry Gas Regulator Replacement		☐ Breath Tube Replacement		☐ Other _____						
Simulator	Serial #	Lot #/Exp																																		
0.050	MP6291	202406K 06/19/2026																																		
0.080	MP6292	202406L 06/19/2026																																		
0.200	MP6293	202406N 06/20/2026																																		
0.080 DGS	N/A	AG325603 09/13/2025																																		
Maintenance By <u>DA</u> Date <u>12/5/24</u>																																				
☐ Battery Replacement																																				
☒ Dry Gas Regulator Replacement																																				
☐ Breath Tube Replacement																																				
☐ Other _____																																				
Calibration Adjustment	By <u>DA</u>		Department Inspection	By <u>DA</u>																																
Barometric Pressure Gauge <u>1016</u> ID # <u>28427</u>			Barometric Pressure ID# <u>28662</u>																																	
<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.000</td><td>MP6294</td><td>N/A</td><td>N/A</td></tr><tr><td>0.040</td><td>MP6295</td><td>24231</td><td>06/25/2026</td></tr><tr><td>0.100</td><td>MP6296</td><td>24110</td><td>03/05/2026</td></tr><tr><td>0.200</td><td>MP6297</td><td>24080</td><td>02/13/2026</td></tr><tr><td>0.300</td><td>MP6298</td><td>24170</td><td>05/07/2026</td></tr><tr><td>0.080 DGS</td><td>N/A</td><td>06723080A5</td><td>04/05/2025</td></tr></tbody></table>	Simulator	Serial #	Lot #	Expiration	0.000	MP6294	N/A	N/A	0.040	MP6295	24231	06/25/2026	0.100	MP6296	24110	03/05/2026	0.200	MP6297	24080	02/13/2026	0.300	MP6298	24170	05/07/2026	0.080 DGS	N/A	06723080A5	04/05/2025			Gauge <u>1012</u> Instrument <u>1011</u>					
Simulator	Serial #	Lot #	Expiration																																	
0.000	MP6294	N/A	N/A																																	
0.040	MP6295	24231	06/25/2026																																	
0.100	MP6296	24110	03/05/2026																																	
0.200	MP6297	24080	02/13/2026																																	
0.300	MP6298	24170	05/07/2026																																	
0.080 DGS	N/A	06723080A5	04/05/2025																																	
☒ Post Calibration Adjustment Stability Checks			Mouth Alcohol Solution Lot # <u>2024-A</u>																																	
<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.050</td><td>MP6291</td><td>202406K</td><td>06/19/2026</td></tr><tr><td>0.080</td><td>MP6292</td><td>202406L</td><td>06/19/2026</td></tr><tr><td>0.200</td><td>MP6293</td><td>202406N</td><td>06/20/2026</td></tr><tr><td>0.080 DGS</td><td>N/A</td><td>AG429602</td><td>10/22/2026</td></tr></tbody></table>	Simulator	Serial #	Lot #	Expiration	0.050	MP6291	202406K	06/19/2026	0.080	MP6292	202406L	06/19/2026	0.200	MP6293	202406N	06/20/2026	0.080 DGS	N/A	AG429602	10/22/2026			Acetone Stock Solution Lot # <u>2023-B</u>													
Simulator	Serial #	Lot #	Expiration																																	
0.050	MP6291	202406K	06/19/2026																																	
0.080	MP6292	202406L	06/19/2026																																	
0.200	MP6293	202406N	06/20/2026																																	
0.080 DGS	N/A	AG429602	10/22/2026																																	
Notes/Suggested Service: <u>AI indicated that the tank psi is 0 with full DGS attached. Performed tank tare to evaluate and instrument still denoted 0psi with DGS attached. Replaced regulator, performed tank tare and evaluated instrument's tank reading. Repeated DGS stability check with nominal results. DA 12/5/24 Tech review: corrected instrument serial number DA 12/16/24</u>			<table border="1"><thead><tr><th>Simulator</th><th>Serial Number</th></tr></thead><tbody><tr><td>0.000</td><td>MP5086</td></tr><tr><td>Interferent</td><td>MP5087</td></tr><tr><td>0.050</td><td>MP5088</td></tr><tr><td>0.080</td><td>MP5089</td></tr><tr><td>0.200</td><td>MP5090</td></tr></tbody></table>	Simulator	Serial Number	0.000	MP5086	Interferent	MP5087	0.050	MP5088	0.080	MP5089	0.200	MP5090																					
Simulator	Serial Number																																			
0.000	MP5086																																			
Interferent	MP5087																																			
0.050	MP5088																																			
0.080	MP5089																																			
0.200	MP5090																																			
			Attachments																																	
			☒ Form 41 ☒ Stability Checks ☒ Calibration Certificate ☒ Calibration Adjustment			☒ Post-Stability Checks ☐ Flow Calibration ☒ Form 40 ☐ Other _____																														
			☒ Instrument Complies with Chapter 11D-8, FAC ☐ Instrument Does Not Comply with Chapter 11D-8, FAC																																	
			☒ Return to/Place into Evidentiary Use ☐ Remain Out of Evidentiary Use																																	
			☒ Conduct an Agency Inspection Before Evidentiary Use																																	
			Taylor Gutschow Digitally signed by Taylor Gutschow Date: 2024.12.18 11:04:39 -05'00'			Shayla Platt Digitally signed by Shayla Platt Date: 2024.12.18 11:28:47 -05'00'																														
			Tech Review / Date _____			Admin Review / Date _____																														

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OKALOOSA COUNTY SO

Time of Inspection: 07:52

Date of Inspection: 12/05/2024

Serial Number: 80-000763

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Number of Simulators Used: _____


Remarks:

BYPASS AI TO OPERATE INSTRUMENT COMPLIANCE NOT DETERMINED

NA- Did not determine Compliance 12/5/24 DA

The above instrument complies (☒) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DESTINEE N ARMSTRONG

Signature and Printed Name

12/05/2024

Date

Stability Checks 80-000763 12/5/24 DA

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
12/05/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	08:10
Control Test	0.049	08:11
Air Blank	0.000	08:11
Control Test	0.048	08:12
Air Blank	0.000	08:12
Control Test	0.049	08:13
Air Blank	0.000	08:13
Control Test Stats		
Average	0.0487	
Std Dev	0.0006	
Rel Std Dev(%)	1.1863	

Operator's Signature

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
12/05/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	08:15
Control Test	0.075	08:15
Air Blank	0.000	08:16
Control Test	0.077	08:17
Air Blank	0.000	08:17
Control Test	0.077	08:18
Air Blank	0.000	08:18
Control Test Stats		
Average	0.0763	
Std Dev	0.0012	
Rel Std Dev(%)	1.5127	

Wet

DA

Operator's Signature

Checked simulator for adequate seal
and performed additional stability check.

12/5/24 DA

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
12/05/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	08:21
Control Test	0.077	08:21
Air Blank	0.000	08:22
Control Test	0.076	08:23
Air Blank	0.000	08:23
Control Test	0.078	08:24
Air Blank	0.000	08:24
Control Test Stats		
Average	0.0770	
Std Dev	0.0010	
Rel Std Dev(%)	1.2987	

Wet


DA

Operator's Signature

Second attempt. 12/5/24 DA

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
12/05/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	08:26
Control Test	0.195	08:27
Air Blank	0.000	08:27
Control Test	0.196	08:28
Air Blank	0.000	08:28
Control Test	0.194	08:29
Air Blank	0.000	08:30
Control Test Stats		
Average	0.1950	
Std Dev	0.0010	
Rel Std Dev(%)	0.5128	



Operator's Signature

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
12/05/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	08:31
Control Test	0.079	08:32
Air Blank	0.000	08:32
Control Test	0.079	08:32
Air Blank	0.000	08:33
Control Test	0.079	08:33
Air Blank	0.000	08:34
Control Test Stats		
Average	0.0790	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

DGS

DA


Operator's Signature

Before ~~changing~~ replacing
DGS regulator. 12/5/24 DA

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
12/05/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	09:10
Control Test	0.079	09:10
Air Blank	0.000	09:11
Control Test	0.079	09:11
Air Blank	0.000	09:11
Control Test	0.079	09:12
Air Blank	0.000	09:12
Control Test Stats		
Average	0.0790	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

DGS



Operator's Signature

After regulator replacement
12/5/24 DA.

Optical Bench Adjustment

12/9/24 DA

OKALOOSA COUNTY SO

Intoxilyzer - Alcohol Analyzer

Model 8000

SN 80-000763

12/09/2024

10:10:18

Auto Calibration

pg 1 of 2

<<<<< 3um >>>>> <<<<< 9um >>>>>

Solution = 0.000 g/210L or 0.0000 mg/l, Samples = 4, Discarded = 1

Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)
Sample #1	0.0000	(0.0000)	0.0000	(0.0000)
Sample #2	0.0000	(0.0000)	0.0000	(0.0000)
Sample #3	0.0000	(0.0000)	0.0000	(0.0000)
Sample #4	0.0000	(0.0000)	0.0000	(0.0000)
Avg % Abs	0.0000	(0.0000)	0.0000	(0.0000)
STD DEV	0.0000	(0.0000)	0.0000	(0.0000)
REL STD DEV	0.000	(0.000)	0.000	(0.000)

Solution = 0.000 g/210L or 0.0000 mg/l, Samples = 4, Discarded = 1

Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)
Sample #1	0.0000	(0.0000)	0.0000	(0.0000)
Sample #2	0.0000	(0.0000)	0.0000	(0.0000)
Sample #3	0.0000	(0.0000)	0.0000	(0.0000)
Sample #4	0.0000	(0.0000)	0.0000	(0.0000)
Avg % Abs	0.0000	(0.0000)	0.0000	(0.0000)
STD DEV	0.0000	(0.0000)	0.0000	(0.0000)
REL STD DEV	0.000	(0.000)	0.000	(0.000)

Solution = 0.000 g/210L or 0.0000 mg/l, Samples = 4, Discarded = 1

Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)
Sample #1	0.0000	(0.0000)	0.0000	(0.0000)
Sample #2	0.0000	(0.0000)	0.0000	(0.0000)
Sample #3	0.0000	(0.0000)	0.0000	(0.0000)
Sample #4	0.0000	(0.0000)	0.0000	(0.0000)
Avg % Abs	0.0000	(0.0000)	0.0000	(0.0000)
STD DEV	0.0000	(0.0000)	0.0000	(0.0000)
REL STD DEV	0.000	(0.000)	0.000	(0.000)

Solution = 0.000 g/210L or 0.0000 mg/l, Samples = 4, Discarded = 1

Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)
Sample #1	0.0000	(0.0000)	0.0000	(0.0000)
Sample #2	0.0000	(0.0000)	0.0000	(0.0000)
Sample #3	0.0000	(0.0000)	0.0000	(0.0000)
Sample #4	0.0000	(0.0000)	0.0000	(0.0000)
Avg % Abs	0.0000	(0.0000)	0.0000	(0.0000)
STD DEV	0.0000	(0.0000)	0.0000	(0.0000)
REL STD DEV	0.000	(0.000)	0.000	(0.000)

Solution = 0.000 g/210L or 0.0000 mg/l, Samples = 4, Discarded = 1

Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)
Sample #1	0.0000	(0.0000)	0.0000	(0.0000)
Sample #2	0.0000	(0.0000)	0.0000	(0.0000)
Sample #3	0.0000	(0.0000)	0.0000	(0.0000)
Sample #4	0.0000	(0.0000)	0.0000	(0.0000)
Avg % Abs	0.0000	(0.0000)	0.0000	(0.0000)
STD DEV	0.0000	(0.0000)	0.0000	(0.0000)
REL STD DEV	0.000	(0.000)	0.000	(0.000)

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
12/09/2024 10:10:18

Auto Calibration

pg 2 of 2

```
<<<<<      3um      >>>>>
-----
Zero Order Coef  -294.94
First Order Coef  2676.76
Second Order Coef 17.55
```

```
-----
Act      Fit      Residual
(g/210L) (g/210L)  (g/210L)
0.000    -0.006    0.0062
0.000    -0.006    0.0062
0.000    -0.006    0.0062
0.000    -0.006    0.0062
0.000    -0.006    0.0062
0.000    -0.006    0.0062
-----
```

```
<<<<<      9um      >>>>>
-----
Zero Order Coef  -221.87
First Order Coef  1384.68
Second Order Coef 11.54
```

```
-----
Act      Fit      Residual
(g/210L) (g/210L)  (g/210L)
0.000    0.000    0.0000
0.000    0.000    0.0000
0.000    0.000    0.0000
0.000    0.000    0.0000
0.000    0.000    0.0000
0.000    0.000    0.0000
-----
```

*****CALIBRATION FAILED*****

Aborted optical bench calibration adjustment
after entering incorrect ethanol concentration.
12/9/24 DA

OKALOOSA COUNTY SO

Intoxilyzer - Alcohol Analyzer

Model 8000

SN 80-000763

12/09/2024

10:15:11

Auto Calibration

pg 1 of 2

<<<<< 3um >>>>>			<<<<< 9um >>>>>		
Solution = 0.000 g/210L or 0.0000 mg/l, Samples = 4, Discarded = 1					
Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)	
Sample #1	0.0840	(-0.0130)	0.1640	(-0.0150)	
Sample #2	0.0850	(0.0020)	0.1220	(-0.0120)	
Sample #3	0.0730	(0.0620)	0.1310	(0.0020)	
Sample #4	0.0840	(0.0770)	0.1530	(0.0120)	
Avg % Abs	0.0807	(0.0470)	0.1353	(0.0007)	
STD DEV	0.0067	(0.0397)	0.0159	(0.0121)	
REL STD DEV	8.254	(84.439)	11.784	(1808.314)	
Solution = 0.040 g/210L or 0.1905 mg/l, Samples = 4, Discarded = 1					
Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)	
Sample #1	0.8080	(-0.0110)	1.4830	(-0.0110)	
Sample #2	0.7920	(-0.0110)	1.4830	(-0.0050)	
Sample #3	0.7860	(0.0350)	1.4930	(0.0030)	
Sample #4	0.7990	(0.0430)	1.4920	(0.0100)	
Avg % Abs	0.7923	(0.0223)	1.4893	(0.0027)	
STD DEV	0.0065	(0.0291)	0.0055	(0.0075)	
REL STD DEV	0.821	(130.492)	0.370	(281.458)	
Solution = 0.100 g/210L or 0.4762 mg/l, Samples = 4, Discarded = 1					
Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)	
Sample #1	1.8850	(-0.0190)	3.4670	(-0.0140)	
Sample #2	1.8690	(0.0130)	3.4560	(0.0050)	
Sample #3	1.8520	(0.0300)	3.4790	(-0.0100)	
Sample #4	1.8520	(0.0300)	3.4660	(0.0030)	
Avg % Abs	1.8577	(0.0243)	3.4670	(-0.0007)	
STD DEV	0.0098	(0.0098)	0.0115	(0.0081)	
REL STD DEV	0.528	(40.335)	0.333	(1221.679)	
Solution = 0.200 g/210L or 0.9524 mg/l, Samples = 4, Discarded = 1					
Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)	
Sample #1	3.5910	(-0.0150)	6.6520	(-0.0020)	
Sample #2	3.5670	(-0.0070)	6.6450	(0.0020)	
Sample #3	3.5770	(0.0200)	6.6310	(0.0190)	
Sample #4	3.5720	(0.0120)	6.6340	(0.0160)	
Avg % Abs	3.5720	(0.0083)	6.6367	(0.0123)	
STD DEV	0.0050	(0.0139)	0.0074	(0.0091)	
REL STD DEV	0.140	(166.421)	0.111	(73.571)	
Solution = 0.300 g/210L or 1.4286 mg/l, Samples = 4, Discarded = 1					
Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)	
Sample #1	5.2680	(-0.0210)	9.6420	(-0.0060)	
Sample #2	5.2450	(0.0230)	9.6110	(0.0330)	
Sample #3	5.2260	(0.0390)	9.6290	(0.0370)	
Sample #4	5.2380	(0.0300)	9.6170	(0.0300)	
Avg % Abs	5.2363	(0.0307)	9.6190	(0.0333)	
STD DEV	0.0096	(0.0080)	0.0092	(0.0035)	
REL STD DEV	0.184	(26.155)	0.095	(10.536)	

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
12/09/2024 10:15:11

Auto Calibration

pg 2 of 2

<<<<< 3um >>>>>

Zero Order Coef -206.75
First Order Coef 2629.58
Second Order Coef 26.36

Act (g/210L)	Fit (g/210L)	Residual (g/210L)
0.000	0.000	-0.0001
0.040	0.040	0.0002
0.100	0.100	-0.0002
0.200	0.200	0.0000
0.300	0.300	0.0000

<<<<< 9um >>>>>

Zero Order Coef -180.09
First Order Coef 1376.99
Second Order Coef 13.13

Act (g/210L)	Fit (g/210L)	Residual (g/210L)
0.000	0.000	-0.0001
0.040	0.040	0.0001
0.100	0.100	0.0002
0.200	0.200	-0.0003
0.300	0.300	0.0001

<<<<< 3um >>>>> <<<<< 9um >>>>>

Solution = 0.080 g/210L or 0.3810 mg/l, Samples = 4, Discarded = 1
Sample
Sample #1 3156.00 3328.00
Sample #2 3055.00 3263.00
Sample #3 3140.00 3306.00
Sample #4 3081.00 3276.00
Avg 3092.0000 3281.6667
STD DEV 43.5546 22.0530
REL STD DEV 1.409 0.672
H2O adjust (mg/l*10k) 717 528


Barometric Pressure = 1015

*****CALIBRATION SUCCESSFUL*****

Post-Stability Checks 80-000763 12/9/24 DA

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
12/09/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	11:12
Control Test	0.050	11:13
Air Blank	0.000	11:13
Control Test	0.049	11:14
Air Blank	0.000	11:14
Control Test	0.049	11:15
Air Blank	0.000	11:16
Control Test Stats		
Average	0.0493	
Std Dev	0.0006	
Rel Std Dev(%)	1.1703	



Operator's Signature

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
12/09/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	11:16
Control Test	0.079	11:17
Air Blank	0.000	11:18
Control Test	0.079	11:18
Air Blank	0.000	11:19
Control Test	0.079	11:20
Air Blank	0.000	11:20
Control Test Stats		
Average	0.0790	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

Wet

DA

Operator's Signature

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
12/09/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	11:27
Control Test	0.199	11:28
Air Blank	0.000	11:28
Control Test	0.199	11:29
Air Blank	0.000	11:30
Control Test	0.199	11:30
Air Blank	0.000	11:31
Control Test Stats		
Average	0.1990	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

DA

Operator's Signature


Repeated this stability check due to
external printer out of paper.

12/9/24 DA

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
12/09/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	11:32
Control Test	0.078	11:32
Air Blank	0.000	11:33
Control Test	0.078	11:33
Air Blank	0.000	11:34
Control Test	0.079	11:34
Air Blank	0.000	11:34
Control Test Stats		
Average	0.0783	
Std Dev	0.0006	
Rel Std Dev(%)	0.7370	

DAS



Operator's Signature

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: OKALOOSA COUNTY SO
Time of Inspection: 13:29

Date of Inspection: 12/10/2024

Serial Number: 80-000763
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202406K Exp: 06/19/2026	0.08g/210L Test (g/210L) Lot#:202406L Exp: 06/19/2026	0.20g/210L Test (g/210L) Lot#:202406N Exp: 06/20/2026	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG429602 Exp: 10/22/2026
0.000	0.049	0.079	0.198	0.079
0.000	0.048	0.079	0.198	0.079
0.000	0.049	0.078	0.198	0.078
0.000	0.049	0.079	0.198	0.079
0.000	0.049	0.078	0.198	0.078
0.000	0.046	0.078	0.198	0.078
0.000	0.049	0.078	0.198	0.079
0.000	0.049	0.079	0.198	0.078
0.000	0.049	0.078	0.198	0.078
0.000	0.049	0.079	0.198	0.079

Standard Deviations	0.0004	0.0005	0.0000	0.0005
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.



I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DESTINEE N ARMSTRONG

Signature and Printed Name

12/10/2024
Date



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
2331 Phillips Road
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-000763 , manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-000763</u>	UNCERTAINTY* $\pm$	
Owning Agency:	<u>OKALOOSA COUNTY SO</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>12/10/2024</u>	0.080 g/ 210 L	0.004
Calibration Time:	<u>13:29</u>	0.200 g/ 210 L	0.007
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.

*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ($k=3$).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards. This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

12/10/2024

Date

DESTINEE N ARMSTRONG,

FDLE/ATP Form 69 October 2024

Issuing Authority: Alcohol Testing Program

Department Inspector

Service • Integrity • Respect • Quality



INSTRUMENT PROCESSING SHEET

Agency Okaloosa County SOS/N 80-000763Florida Department of
Law EnforcementDate In 06/26/2024 DI Completion Date 7/2/2024☒ Ship ☐ P/U ☐ H/D ☐ CMI ☐ EE

Intake By <u>ALL</u> Date <u>06/26/2024</u>	Quality Checks By <u>ALL</u> Date <u>07/01/2024</u>	Flow Calibration By _____ Date _____																																																												
☒ Annual ☐ Registration ☐ Return from CMI / EE Visual Inspection: ☒ Case ☒ Handle ☒ Keyboard ☒ Dry Gas Shelf ☒ Feet ☒ Breath Tube ☒ Ports ☒ Screws Tight Other Equipment/ Accessories: ☐ Power cord ☐ Printer Cable ☐ Static Bag ☐ 12V DC Cable Notes: instrument arrived in FDLE box and with panel on inlet side unattached	☒ Breath Tube Screen ☒ Replace External O-Rings ☒ Instrument Set Up Verified ☒ R-Value <u>207</u> ☒ Flow Verification (L/s) Flow Column # <u>ATP-103</u> 32 mm <u>.144</u> (.139 - .169) 36 mm <u>.167</u> (.156 - .190) 53 mm <u>.238</u> (.228 - .278) 103 mm <u>.496</u> (.447 - .547) ☒ Barometric Pressure Check Gauge ID # <u>28662</u> ☒ Stability Checks <table border="1" style="width:100%; border-collapse: collapse;"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #/Exp</th></tr></thead><tbody><tr><td>0.050</td><td>MP5088</td><td>202303K 03/29/2025</td></tr><tr><td>0.080</td><td>MP5089</td><td>202303L 03/29/2025</td></tr><tr><td>0.200</td><td>MP5090</td><td>202304C 04/05/2025</td></tr><tr><td>0.080 DGS</td><td>N/A</td><td>AG310901 04/19/2025</td></tr></tbody></table>	Simulator	Serial #	Lot #/Exp	0.050	MP5088	202303K 03/29/2025	0.080	MP5089	202303L 03/29/2025	0.200	MP5090	202304C 04/05/2025	0.080 DGS	N/A	AG310901 04/19/2025	Flow Column # _____ ☐ 5L/min – 17mm ☐ 15L/min – 53mm ☐ 30L/min – 103mm ☐ R-Value _____ ☐ Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547) Maintenance By _____ Date _____ ☐ Battery Replacement ☐ Dry Gas Regulator Replacement ☐ Breath Tube Replacement ☐ Other _____																																													
Simulator	Serial #	Lot #/Exp																																																												
0.050	MP5088	202303K 03/29/2025																																																												
0.080	MP5089	202303L 03/29/2025																																																												
0.200	MP5090	202304C 04/05/2025																																																												
0.080 DGS	N/A	AG310901 04/19/2025																																																												
Calibration Adjustment By _____		Department Inspection By <u>SP</u>																																																												
Barometric Pressure Gauge _____ ID # _____ <table border="1" style="width:100%; border-collapse: collapse;"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.000</td><td></td><td>N/A</td><td>N/A</td></tr><tr><td>0.040</td><td></td><td></td><td></td></tr><tr><td>0.100</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.300</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table> ☐ Post Calibration Adjustment Stability Checks <table border="1" style="width:100%; border-collapse: collapse;"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.050</td><td></td><td></td><td></td></tr><tr><td>0.080</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table>		Simulator	Serial #	Lot #	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Simulator	Serial #	Lot #	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			Barometric Pressure ID# <u>28421</u> Gauge <u>1014</u> Instrument <u>1015</u> Mouth Alcohol Solution Lot # <u>2024-A</u> Acetone Stock Solution Lot # <u>2023-B</u> <table border="1" style="width:100%; border-collapse: collapse;"><thead><tr><th>Simulator</th><th>Serial Number</th></tr></thead><tbody><tr><td>0.000</td><td>MP5086</td></tr><tr><td>Interferent</td><td>MP5087</td></tr><tr><td>0.050</td><td>MP5088</td></tr><tr><td>0.080</td><td>MP5089</td></tr><tr><td>0.200</td><td>MP5090</td></tr></tbody></table> Attachments ☒ Form 41 ☒ Stability Checks ☒ Calibration Certificate ☐ Calibration Adjustment ☐ Post-Stability Checks ☐ Flow Calibration ☐ Form 40 ☐ Other _____ ☒ Instrument Complies with Chapter 11D-8, FAC ☐ Instrument Does Not Comply with Chapter 11D-8, FAC ☒ Return to/Place into Evidentiary Use ☐ Remain Out of Evidentiary Use ☒ Conduct an Agency Inspection Before Evidentiary Use	Simulator	Serial Number	0.000	MP5086	Interferent	MP5087	0.050	MP5088	0.080	MP5089	0.200	MP5090
Simulator	Serial #	Lot #	Expiration																																																											
0.000		N/A	N/A																																																											
0.040																																																														
0.100																																																														
0.200																																																														
0.300																																																														
0.080 DGS	N/A																																																													
Simulator	Serial #	Lot #	Expiration																																																											
0.050																																																														
0.080																																																														
0.200																																																														
0.080 DGS	N/A																																																													
Simulator	Serial Number																																																													
0.000	MP5086																																																													
Interferent	MP5087																																																													
0.050	MP5088																																																													
0.080	MP5089																																																													
0.200	MP5090																																																													
Notes/Suggested Service: _____ Tech Review : added notes and initial to stability check page. SP 7/9/24 Exhaust port cover received and placed on instrument 7/15/24 prior to return to agency. SP 7/15/24		Taylor Gutschow Digitally signed by Taylor Gutschow Date: 2024.07.09 15:09:24 +04'00' Phil Nicodemo Digitally signed by Phil Nicodemo Date: 2024.07.12 11:19:31 -04'00' Tech Review / Date _____ Admin Review / Date _____																																																												

Stability Checks 80-000763

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
07/01/2024
Software: 8100.27

Test	g/210L	Time
Air Blank		
Control Test	0.049	10:22
Air Blank		10:23
Control Test	0.049	10:24
Air Blank	0.000	10:24
Control Test	0.049	10:25
Air Blank	0.000	10:25
Control Test Stats		
Average	0.0490	
Std Dev	0.0070	
Rel Std Dev(%)	0.0009	

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
07/01/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	10:29
Control Test	0.078	10:30
Air Blank	0.000	10:30
Control Test	0.077	10:31
Air Blank	0.000	10:32
Control Test	0.078	10:32
Air Blank	0.000	10:33
Control Test Stats		
Average	0.0777	
Std Dev	0.0006	
Rel Std Dev(%)	0.7434	

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
07/01/2024
Software: 8100.27

Test	g/210L	Time
Air Blank		10:37
Control Test	0.154	10:38
Air Blank	0.000	10:38
Control Test	0.153	10:39
Air Blank	0.000	10:39
Control Test	0.191	10:40
Air Blank	0.000	10:41
Control Test Stats		
Average	0.1505	
Std Dev	0.0015	
Rel Std Dev(%)	0.7928	

Wet

SP
7/2/24
sim jar
chipped SP

Initials added 7/9/24

Operator's Signature

Operator's Signature

Operator's Signature

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
07/01/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	07:18
Control Test	0.195	07:18
Air Blank	0.000	07:19
Control Test	0.195	07:19
Air Blank	0.000	07:20
Control Test	0.196	07:21
Air Blank	0.000	07:21
Control Test Stats		
Average	0.1953	
Std Dev	0.0006	
Rel Std Dev(%)	0.2956	

OKALOOSA COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000763
07/01/2024
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	10:52
Control Test	0.079	10:53
Air Blank	0.000	10:53
Control Test	0.076	10:53
Air Blank	0.000	10:53
Control Test	0.078	10:54
Air Blank	0.000	10:54
Control Test Stats		
Average	0.0783	
Std Dev	0.0006	
Rel Std Dev(%)	0.7370	

D65

Operator's Signature

Operator's Signature

Repeated 0.200 stability check with new sim jar. SP
repeat stability conducted on 7/2/24. SP
7/9/24

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: OKALOOSA COUNTY SO
Time of Inspection: 09:09

Date of Inspection: 07/02/2024

Serial Number: 80-000763
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303K Exp: 03/29/2025	0.08g/210L Test (g/210L) Lot#:202303L Exp: 03/29/2025	0.20g/210L Test (g/210L) Lot#:202304C Exp: 04/05/2025	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG310901 Exp: 04/19/2025
0.000	0.049	0.077	0.197	0.078
0.000	0.048	0.077	0.196	0.078
0.000	0.048	0.077	0.197	0.078
0.000	0.048	0.078	0.196	0.078
0.000	0.048	0.078	0.196	0.078
0.000	0.048	0.078	0.197	0.078
0.000	0.049	0.078	0.197	0.078
0.000	0.049	0.077	0.196	0.078
0.000	0.049	0.078	0.197	0.078
0.000	0.048	0.077	0.196	0.078
Standard Deviations	0.0005	0.0005	0.0005	0.0000

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

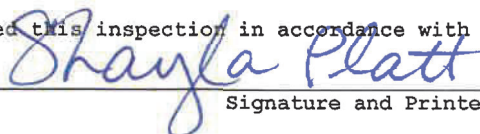

SHAYLA D PLATT

Signature and Printed Name

07/02/2024
Date



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
2331 Phillips Road.
Suite B1032
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-000763, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-000763</u>	UNCERTAINTY* $\pm$	
Owning Agency:	<u>OKALOOSA COUNTY SO</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>07/02/2024</u>	0.080 g/ 210 L	0.004
Calibration Time:	<u>09:09</u>	0.200 g/ 210 L	0.007
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.

*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ($k=3$).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards.

This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

Shayla
Platt
Digitally signed by
Shayla Platt
Date: 2024.07.05
19:38:55 -04'00'

07/02/2024

Date

SHAYLA D PLATT,

Department Inspector

FDLE/ATP Form 69 March 2022
Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality