



INSTRUMENT PROCESSING SHEET

Agency GULF BREEZE PDS/N 80-001306Florida Department of
Law EnforcementDate In 7/8/25DI Completion Date 07/17/2025☒ Ship ☐ P/U ☐ H/D ☐ CMI ☐ EE

Intake	By KTS	Date 7/8/25	Quality Checks	By KTS	Date 7/8/25	Flow Calibration	By	Date																											
☒ Annual ☐ Registration ☐ Return from CMI / EE Visual Inspection: ☒ Case ☐ Handle ☒ Keyboard ☐ Dry Gas Shelf ☒ Feet ☐ Breath Tube ☒ Ports ☐ Screws Tight Other Equipment/ Accessories: ☐ Power cord ☐ Printer Cable ☒ Static Bag ☐ 12V DC Cable Notes: <u>Note from Agency</u> <u>Inspector. KTS 7/8/25</u>			☒ Breath Tube Screen ☒ Replace External O-Rings ☒ Instrument Set Up Verified ☒ R-Value <u>235</u> ☒ Flow Verification (L/s) Flow Column # <u>ATP103</u> 32 mm <u>0.148</u> (.139 - .169) 36 mm <u>0.160</u> (.156 - .190) 53 mm <u>0.242</u> (.228 - .278) 103 mm <u>0.484</u> (.447 - .547) ☒ Barometric Pressure Check Gauge ID # <u>28427</u> ☒ Stability Checks			Flow Column # _____ ☐ 5L/min – 17mm ☐ 15L/min – 53mm ☐ 30L/min – 103mm ☐ R-Value _____ ☐ Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547)																													
			<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #/Exp</th></tr></thead><tbody><tr><td>0.050</td><td>MP5088</td><td>202406K 6/19/26</td></tr><tr><td>0.080</td><td>MP5089</td><td>202406L 6/19/26</td></tr><tr><td>0.200</td><td>MP5090</td><td>202406N 6/20/26</td></tr><tr><td>0.080 DGS</td><td>N/A</td><td>AG429602 10/22/26</td></tr></tbody></table>	Simulator	Serial #	Lot #/Exp	0.050	MP5088	202406K 6/19/26	0.080	MP5089	202406L 6/19/26	0.200	MP5090	202406N 6/20/26	0.080 DGS	N/A	AG429602 10/22/26																	
Simulator	Serial #	Lot #/Exp																																	
0.050	MP5088	202406K 6/19/26																																	
0.080	MP5089	202406L 6/19/26																																	
0.200	MP5090	202406N 6/20/26																																	
0.080 DGS	N/A	AG429602 10/22/26																																	
Calibration Adjustment By _____			Department Inspection By <u>SLH</u>																																
Barometric Pressure Gauge _____ ID # _____			Barometric Pressure ID# <u>28421</u>																																
<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.000</td><td></td><td>N/A</td><td>N/A</td></tr><tr><td>0.040</td><td></td><td></td><td></td></tr><tr><td>0.100</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.300</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table>			Simulator	Serial #	Lot #	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Gauge <u>1017</u> Instrument <u>1015</u> Mouth Alcohol Solution Lot # <u>2025-A</u> Acetone Stock Solution Lot # <u>2024-B</u>				
Simulator	Serial #	Lot #	Expiration																																
0.000		N/A	N/A																																
0.040																																			
0.100																																			
0.200																																			
0.300																																			
0.080 DGS	N/A																																		
☐ Post Calibration Adjustment Stability Checks			<table border="1"><thead><tr><th>Simulator</th><th>Serial Number</th></tr></thead><tbody><tr><td>0.000</td><td>MP6294</td></tr><tr><td>Interferent</td><td>MP5087</td></tr><tr><td>0.050</td><td>MP5088</td></tr><tr><td>0.080</td><td>MP5089</td></tr><tr><td>0.200</td><td>MP5090</td></tr></tbody></table>					Simulator	Serial Number	0.000	MP6294	Interferent	MP5087	0.050	MP5088	0.080	MP5089	0.200	MP5090																
Simulator	Serial Number																																		
0.000	MP6294																																		
Interferent	MP5087																																		
0.050	MP5088																																		
0.080	MP5089																																		
0.200	MP5090																																		
<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.050</td><td></td><td></td><td></td></tr><tr><td>0.080</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table>			Simulator	Serial #	Lot #	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			Attachments ☒ Form 41 ☐ Post-Stability Checks ☒ Stability Checks ☐ Flow Calibration ☒ Calibration Certificate ☐ Form 40 ☐ Calibration Adjustment ☒ Other <u>Agency note</u>												
Simulator	Serial #	Lot #	Expiration																																
0.050																																			
0.080																																			
0.200																																			
0.080 DGS	N/A																																		
Notes/Suggested Service: <u>Returning with cord. KTS 7/8/25</u>			☒ Instrument Complies with Chapter 11D-8, FAC ☐ Instrument Does Not Comply with Chapter 11D-8, FAC ☒ Return to/Place into Evidentiary Use ☐ Remain Out of Evidentiary Use ☒ Conduct an Agency Inspection Before Evidentiary Use																																
			Shayla Platt Digitally signed by Shayla Platt Date: 2025.07.29 09:40:27 -04'00'																																
			Tech Review / Date _____ Admiri Review / Date _____																																

1306


There was a black power cord sent with the last intoxilyzer that Gulf Breeze Police Department sent. Upon return the black power cable was not in the box with the intoxilyzer. Please send us back the other black power cord connected to this intoxilyzer. As you will notice, this intoxilyzer does not have a black power cord, and that is because I had to take it off and use it with the spare one you sent back to us. I would also like to request a new box for the intoxilyzer and new foam to mail it to you with. Thank you for your attention to this matter.

If there are any issues, you can call my personal phone at 8507765164, or email me at dhart@gulfbreezefl.gov

Officer Dylan Hart, Gulf Breeze Police Department

GULF BREEZE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001306
07/08/2025
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	13:37
Control Test	0.077	13:37
Air Blank	0.000	13:38
Control Test	0.077	13:38
Air Blank	0.000	13:39
Control Test	0.077	13:39
Air Blank	0.000	13:39
Control Test Stats		
Average	0.0770	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

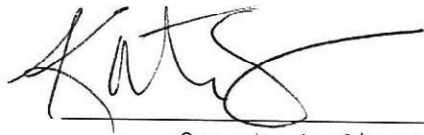


Operator's Signature

Dry

GULF BREEZE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001306
07/08/2025
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	13:44
Control Test	0.049	13:44
Air Blank	0.000	13:45
Control Test	0.049	13:46
Air Blank	0.000	13:46
Control Test	0.049	13:47
Air Blank	0.000	13:48
Control Test Stats		
Average	0.0490	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

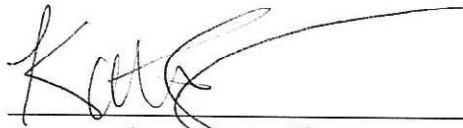
Operator's Signature

GULF BREEZE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001306
07/08/2025
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	13:49
Control Test	0.079	13:49
Air Blank	0.000	13:50
Control Test	0.078	13:51
Air Blank	0.000	13:51
Control Test	0.079	13:52
Air Blank	0.000	13:52
Control Test Stats		
Average	0.0787	
Std Dev	0.0006	
Rel Std Dev(%)	0.7339	



Operator's Signature

GULF BREEZE PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001306
07/08/2025
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	13:55
Control Test	0.199	13:56
Air Blank	0.000	13:57
Control Test	0.199	13:57
Air Blank	0.000	13:58
Control Test	0.198	13:58
Air Blank	0.000	13:59
Control Test Stats		
Average	0.1987	
Std Dev	0.0006	
Rel Std Dev(%)	0.2906	



Operator's Signature

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: GULF BREEZE PD
Time of Inspection: 13:33

Date of Inspection: 07/08/2025

Serial Number: 80-001306
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08g/210L Test (g/210L) Lot#:_____ Exp:_____	0.20g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:_____ Exp:_____

Number of Simulators Used: _____

Remarks:

BYPASSED AI TO OPERATE. COMPLIANCE NOT DETERMINED.

The above instrument complies (☒) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



KATIE T SPEARIN
Signature and Printed Name

07/08/2025
Date

Florida Department of Law Enforcement

Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: GULF BREEZE PD
Time of Inspection: 15:34

Date of Inspection: 07/17/2025

Serial Number: 80-001306
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202406K Exp: 06/19/2026	0.08g/210L Test (g/210L) Lot#:202406L Exp: 06/19/2026	0.20g/210L Test (g/210L) Lot#:202406N Exp: 06/20/2026	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG429602 Exp: 10/22/2026
0.000	0.048	0.079	0.198	0.077
0.000	0.047	0.079	0.198	0.077
0.000	0.048	0.079	0.199	0.077
0.000	0.048	0.079	0.198	0.077
0.000	0.049	0.079	0.199	0.078
0.000	0.048	0.079	0.199	0.077
0.000	0.049	0.079	0.199	0.077
0.000	0.048	0.079	0.199	0.077
0.000	0.048	0.080	0.199	0.077
0.000	0.048	0.079	0.199	0.077


Standard Deviations	0.0005	0.0003	0.0004	0.0003
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.


I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



LEANDRA HIGGINBOTHAM

Signature and Printed Name

07/17/2025
Date



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
2331 Phillips Road
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-001306, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-001306</u>	UNCERTAINTY* $\pm$	
Owning Agency:	<u>GULF BREEZE PD</u>	0.050 g/210 L	0.004
Calibration Date:	<u>07/17/2025</u>	0.080 g/210 L	0.004
Calibration Time:	<u>15:34</u>	0.200 g/210 L	0.007
		0.080 g/210 L Dry Gas Control	0.005

All results are reported in g/210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 3%, whichever is greater, of the target alcohol concentration.

*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ($k=3$).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/IEC 17025 standards.

This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

07/17/2025

Date

LEANDRA HIGGINBOTHAM,

Department Inspector

FDLE/ATP Form 69 October 2024

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality