





INSTRUMENT PROCESSING SHEET

Agency FHPS/N 80-006768Florida Department of
Law EnforcementDate In 6/27/2025DI Completion Date 07/09/2025☐ Ship ☒ P/U ☐ H/D ☐ CMI ☐ EE

Intake	By SLH	Date <u>6/27/2025</u>	Quality Checks	By KTS	Date <u>7/2/25</u>	Flow Calibration	By SLH	Date <u>07/07/2025</u>																																																																	
☒ Annual ☐ Registration ☐ Return from CMI / EE Visual Inspection: ☒ Case ☒ Handle ☒ Keyboard ☒ Dry Gas Shelf ☒ Feet ☒ Breath Tube ☒ Ports ☒ Screws Tight Other Equipment/ Accessories: ☐ Power cord ☐ Printer Cable ☐ Static Bag ☐ 12V DC Cable Notes: <u>Dropped off by Susan Barge.SLH</u>			☒ Breath Tube Screen ☒ Replace External O-Rings ☒ Instrument Set Up Verified ☒ R-Value <u>135</u> ☒ Flow Verification (L/s) Flow Column # <u>ATP102</u> 32 mm <u>0.136</u> (.139 - .169) 36 mm <u>0.152</u> (.156 - .190) 53 mm <u>0.226</u> (.228 - .278) 103 mm <u>0.500</u> (.447 - .547) ☒ Barometric Pressure Check Gauge ID # <u>28421</u> ☒ Stability Checks			Flow Column # <u>ATP103</u> ☒ 5L/min – 17mm ☒ 15L/min – 53mm ☒ 30L/min – 103mm ☒ R-Value <u>137</u> ☒ Post Calibration Verification (L/s) Flow Column # <u>ATP102</u> 32 mm <u>0.148</u> (.139 - .169) 36 mm <u>0.167</u> (.156 - .190) 53 mm <u>0.234</u> (.228 - .278) 103 mm <u>0.496</u> (.447 - .547)																																																																			
			<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #/Exp</th></tr></thead><tbody><tr><td>0.050</td><td>MP5088</td><td>202406K 6/19/26</td></tr><tr><td>0.080</td><td>MP5089</td><td>202406L 6/19/26</td></tr><tr><td>0.200</td><td>MP5090</td><td>202406N 6/20/26</td></tr><tr><td>0.080 DGS</td><td>N/A</td><td>AG429602 10/22/26</td></tr></tbody></table>			Simulator	Serial #	Lot #/Exp	0.050	MP5088	202406K 6/19/26	0.080	MP5089	202406L 6/19/26	0.200	MP5090	202406N 6/20/26	0.080 DGS	N/A	AG429602 10/22/26	<table border="1"><thead><tr><th colspan="2">Maintenance By _____ Date _____</th></tr></thead><tbody><tr><td colspan="2">☐ Battery Replacement</td></tr><tr><td colspan="2">☐ Dry Gas Regulator Replacement</td></tr><tr><td colspan="2">☐ Breath Tube Replacement</td></tr><tr><td colspan="2">☐ Other _____</td></tr></tbody></table>			Maintenance By _____ Date _____		☐ Battery Replacement		☐ Dry Gas Regulator Replacement		☐ Breath Tube Replacement		☐ Other _____																																									
Simulator	Serial #	Lot #/Exp																																																																							
0.050	MP5088	202406K 6/19/26																																																																							
0.080	MP5089	202406L 6/19/26																																																																							
0.200	MP5090	202406N 6/20/26																																																																							
0.080 DGS	N/A	AG429602 10/22/26																																																																							
Maintenance By _____ Date _____																																																																									
☐ Battery Replacement																																																																									
☐ Dry Gas Regulator Replacement																																																																									
☐ Breath Tube Replacement																																																																									
☐ Other _____																																																																									
Calibration Adjustment By _____			Department Inspection By <u>SLH</u>																																																																						
Barometric Pressure Gauge _____ ID # _____ <table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.000</td><td></td><td>N/A</td><td>N/A</td></tr><tr><td>0.040</td><td></td><td></td><td></td></tr><tr><td>0.100</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.300</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table> ☐ Post Calibration Adjustment Stability Checks <table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.050</td><td></td><td></td><td></td></tr><tr><td>0.080</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table>			Simulator	Serial #	Lot #	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Simulator	Serial #	Lot #	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			Barometric Pressure ID# <u>28662</u> Gauge <u>1015</u> Instrument <u>1017</u> Mouth Alcohol Solution Lot # <u>2025-A</u> Acetone Stock Solution Lot # <u>2024-B</u> <table border="1"><thead><tr><th>Simulator</th><th>Serial Number</th></tr></thead><tbody><tr><td>0.000</td><td>MP6294</td></tr><tr><td>Interferent</td><td>MP5087</td></tr><tr><td>0.050</td><td>MP5088</td></tr><tr><td>0.080</td><td>MP5089</td></tr><tr><td>0.200</td><td>MP5090</td></tr></tbody></table> Attachments <table border="1"><tbody><tr><td>☒ Form 41</td><td>☐ Post-Stability Checks</td></tr><tr><td>☒ Stability Checks</td><td>☒ Flow Calibration</td></tr><tr><td>☒ Calibration Certificate</td><td>☐ Form 40</td></tr><tr><td>☐ Calibration Adjustment</td><td>☐ Other _____</td></tr></tbody></table> ☒ Instrument Complies with Chapter 11D-8, FAC ☐ Instrument Does Not Comply with Chapter 11D-8, FAC ☒ Return to/Place into Evidentiary Use ☐ Remain Out of Evidentiary Use ☒ Conduct an Agency Inspection Before Evidentiary Use Digitally signed by Taylor Gutschow Date: 2025.07.16 13:43:38 -0400 Taylor Gutschow Digitally signed by Shayla Platt Date: 2025.07.16 14:49:51 -0400 Shayla Platt Tech Review / Date _____ Admin Review / Date _____			Simulator	Serial Number	0.000	MP6294	Interferent	MP5087	0.050	MP5088	0.080	MP5089	0.200	MP5090	☒ Form 41	☐ Post-Stability Checks	☒ Stability Checks	☒ Flow Calibration	☒ Calibration Certificate	☐ Form 40	☐ Calibration Adjustment	☐ Other _____
Simulator	Serial #	Lot #	Expiration																																																																						
0.000		N/A	N/A																																																																						
0.040																																																																									
0.100																																																																									
0.200																																																																									
0.300																																																																									
0.080 DGS	N/A																																																																								
Simulator	Serial #	Lot #	Expiration																																																																						
0.050																																																																									
0.080																																																																									
0.200																																																																									
0.080 DGS	N/A																																																																								
Simulator	Serial Number																																																																								
0.000	MP6294																																																																								
Interferent	MP5087																																																																								
0.050	MP5088																																																																								
0.080	MP5089																																																																								
0.200	MP5090																																																																								
☒ Form 41	☐ Post-Stability Checks																																																																								
☒ Stability Checks	☒ Flow Calibration																																																																								
☒ Calibration Certificate	☐ Form 40																																																																								
☐ Calibration Adjustment	☐ Other _____																																																																								
Notes/Suggested Service: <u>Root cause analysis (RCA) performed, DGS was not attached to port. RCA for flow no user or equipment error determined. KTS 7/2/25</u>																																																																									


Stability Checks

0.050 g/210L	0.080 g/210L	0.200 g/210L	DGS 0.080 g/210L																																																																																																																																																
0.047 to 0.053 g/210L ☒	0.077 to 0.083 g/210L ☒	0.194 to 0.206 g/210L ☐	0.077 to 0.083 g/210L ☒ ≤0.003 g/210L of Wet ☒																																																																																																																																																
Performed Root Case Analysis ☐	Performed Root Case Analysis ☐	Performed Root Case Analysis ☐	Performed Root Case Analysis ☒																																																																																																																																																
placed mark 7/14/25 SLH																																																																																																																																																			
FL HIGHWAY PATROL Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-006768 07/02/2025 Software: 8100.27 <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>06:48</td></tr> <tr><td>Control Test</td><td>0.048</td><td>06:48</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>06:49</td></tr> <tr><td>Control Test</td><td>0.048</td><td>06:49</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>06:50</td></tr> <tr><td>Control Test</td><td>0.049</td><td>06:51</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>06:51</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0483</td><td></td></tr> <tr><td>Std Dev</td><td>0.0006</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>1.1945</td><td></td></tr> </tbody> </table>  Operator's Signature	Test	g/210L	Time	Air Blank	0.000	06:48	Control Test	0.048	06:48	Air Blank	0.000	06:49	Control Test	0.048	06:49	Air Blank	0.000	06:50	Control Test	0.049	06:51	Air Blank	0.000	06:51	Control Test Stats			Average	0.0483		Std Dev	0.0006		Rel Std Dev(%)	1.1945		FL HIGHWAY PATROL Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-006768 07/02/2025 Software: 8100.27 <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>06:57</td></tr> <tr><td>Control Test</td><td>0.079</td><td>06:58</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>06:58</td></tr> <tr><td>Control Test</td><td>0.079</td><td>06:59</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>06:59</td></tr> <tr><td>Control Test</td><td>0.079</td><td>07:00</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>07:01</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0790</td><td></td></tr> <tr><td>Std Dev</td><td>0.0000</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>0.0000</td><td></td></tr> </tbody> </table>  Operator's Signature	Test	g/210L	Time	Air Blank	0.000	06:57	Control Test	0.079	06:58	Air Blank	0.000	06:58	Control Test	0.079	06:59	Air Blank	0.000	06:59	Control Test	0.079	07:00	Air Blank	0.000	07:01	Control Test Stats			Average	0.0790		Std Dev	0.0000		Rel Std Dev(%)	0.0000		FL HIGHWAY PATROL Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-006768 07/02/2025 Software: 8100.27 <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>07:02</td></tr> <tr><td>Control Test</td><td>0.200</td><td>07:02</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>07:03</td></tr> <tr><td>Control Test</td><td>0.200</td><td>07:04</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>07:04</td></tr> <tr><td>Control Test</td><td>0.200</td><td>07:05</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>07:05</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.2000</td><td></td></tr> <tr><td>Std Dev</td><td>0.0000</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>0.0000</td><td></td></tr> </tbody> </table>  Operator's Signature	Test	g/210L	Time	Air Blank	0.000	07:02	Control Test	0.200	07:02	Air Blank	0.000	07:03	Control Test	0.200	07:04	Air Blank	0.000	07:04	Control Test	0.200	07:05	Air Blank	0.000	07:05	Control Test Stats			Average	0.2000		Std Dev	0.0000		Rel Std Dev(%)	0.0000		FL HIGHWAY PATROL Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-006768 07/02/2025 Software: 8100.27 <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>06:52</td></tr> <tr><td>Control Test</td><td>0.077</td><td>06:53</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>06:53</td></tr> <tr><td>Control Test</td><td>0.077</td><td>06:53</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>06:54</td></tr> <tr><td>Control Test</td><td>0.077</td><td>06:54</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>06:55</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0770</td><td></td></tr> <tr><td>Std Dev</td><td>0.0000</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>0.0000</td><td></td></tr> </tbody> </table>  Operator's Signature	Test	g/210L	Time	Air Blank	0.000	06:52	Control Test	0.077	06:53	Air Blank	0.000	06:53	Control Test	0.077	06:53	Air Blank	0.000	06:54	Control Test	0.077	06:54	Air Blank	0.000	06:55	Control Test Stats			Average	0.0770		Std Dev	0.0000		Rel Std Dev(%)	0.0000	
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	06:48																																																																																																																																																	
Control Test	0.048	06:48																																																																																																																																																	
Air Blank	0.000	06:49																																																																																																																																																	
Control Test	0.048	06:49																																																																																																																																																	
Air Blank	0.000	06:50																																																																																																																																																	
Control Test	0.049	06:51																																																																																																																																																	
Air Blank	0.000	06:51																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0483																																																																																																																																																		
Std Dev	0.0006																																																																																																																																																		
Rel Std Dev(%)	1.1945																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	06:57																																																																																																																																																	
Control Test	0.079	06:58																																																																																																																																																	
Air Blank	0.000	06:58																																																																																																																																																	
Control Test	0.079	06:59																																																																																																																																																	
Air Blank	0.000	06:59																																																																																																																																																	
Control Test	0.079	07:00																																																																																																																																																	
Air Blank	0.000	07:01																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0790																																																																																																																																																		
Std Dev	0.0000																																																																																																																																																		
Rel Std Dev(%)	0.0000																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	07:02																																																																																																																																																	
Control Test	0.200	07:02																																																																																																																																																	
Air Blank	0.000	07:03																																																																																																																																																	
Control Test	0.200	07:04																																																																																																																																																	
Air Blank	0.000	07:04																																																																																																																																																	
Control Test	0.200	07:05																																																																																																																																																	
Air Blank	0.000	07:05																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.2000																																																																																																																																																		
Std Dev	0.0000																																																																																																																																																		
Rel Std Dev(%)	0.0000																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	06:52																																																																																																																																																	
Control Test	0.077	06:53																																																																																																																																																	
Air Blank	0.000	06:53																																																																																																																																																	
Control Test	0.077	06:53																																																																																																																																																	
Air Blank	0.000	06:54																																																																																																																																																	
Control Test	0.077	06:54																																																																																																																																																	
Air Blank	0.000	06:55																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0770																																																																																																																																																		
Std Dev	0.0000																																																																																																																																																		
Rel Std Dev(%)	0.0000																																																																																																																																																		

RCA for the 0.080g/210L dry gas standard see IPS-
SLH 7/14/25

FL HIGHWAY PATROL
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-006768
07/02/2025
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	06:41
Control Test	0.000	06:41
Air Blank	0.000	06:42
Control Test	0.000	06:42
Air Blank	0.000	06:42
Control Test	0.000	06:43
Air Blank	0.000	06:43
Control Test Stats		
Average	0.0000	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

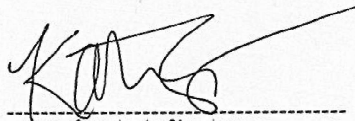

Operator's Signature

Flow Calibration

80-006768

SLH

Root Cause Analysis Performed Prior

Performed by SLH



See note
on IPS

SLH

7/7/25

INTOXILYZER 8000
Instrument Initialization
12:44 07/07/2025

FL HIGHWAY PATROL
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-006768
07/07/2025
Software: 8100.27

Flow Rate Calibration*****

1: Rate (Liters/min) = 5

SQRT(Diff)) = 6.855

2: Rate (Liters/min) = 15

SQRT(Diff)) = 11.398

3: Rate (Liters/min) = 30

SQRT(Diff)) = 21.234

Dependent Data Scale Factor = 100000 L/min

Independent Data Scale Factor = 256

Rounded Slope = 666

Rounded Intercept = -576720

Correlation = 0.99554

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 15:38

Date of Inspection: 07/09/2025

Serial Number: 80-006768
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202406K Exp: 06/19/2026	0.08g/210L Test (g/210L) Lot#:202406L Exp: 06/19/2026	0.20g/210L Test (g/210L) Lot#:202406N Exp: 06/20/2026	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG429602 Exp: 10/22/2026
0.000	0.048	0.079	0.199	0.077
0.000	0.048	0.079	0.198	0.077
0.000	0.048	0.080	0.199	0.077
0.000	0.048	0.080	0.199	0.077
0.000	0.047	0.079	0.198	0.077
0.000	0.048	0.080	0.198	0.077
0.000	0.048	0.080	0.198	0.077
0.000	0.048	0.080	0.199	0.077
0.000	0.048	0.080	0.199	0.077
0.000	0.048	0.080	0.198	0.077


Standard Deviations	0.0003	0.0004	0.0005	0.0000
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5

Remarks:



The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



LEANDRA HIGGINBOTHAM
Signature and Printed Name

07/09/2025
Date



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
2331 Phillips Road
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-006768, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-006768</u>	UNCERTAINTY* $\pm$
Owning Agency:	<u>FL HIGHWAY PATROL</u>	0.050 g/ 210 L 0.004
Calibration Date:	<u>07/09/2025</u>	0.080 g/ 210 L 0.004
Calibration Time:	<u>15:38</u>	0.200 g/ 210 L 0.007
		0.080 g/ 210 L Dry Gas Control 0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.

*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ($k=3$).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards. This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

FDLE/ATP Form 69 October 2024

Issuing Authority: Alcohol Testing Program

Date

07/09/2025

LEANDRA HIGGINBOTHAM,

Department Inspector

Service • Integrity • Respect • Quality