



INSTRUMENT PROCESSING SHEET

Agency Marion County SOS/N 80-000827Florida Department of
Law EnforcementDate In 5/22/2025DI Completion Date 6/3/2025 Ship P/U H/D CMI EE

Intake By <u>SLH</u> Date <u>06/02/2025</u> <input checked="" type="checkbox"/> Annual <input type="checkbox"/> Registration <input type="checkbox"/> Return from CMI / EE Visual Inspection: <input checked="" type="checkbox"/> Case <input checked="" type="checkbox"/> Handle <input checked="" type="checkbox"/> Keyboard <input checked="" type="checkbox"/> Dry Gas Shelf <input checked="" type="checkbox"/> Feet <input checked="" type="checkbox"/> Breath Tube <input checked="" type="checkbox"/> Ports <input checked="" type="checkbox"/> Screws Tight Other Equipment/ Accessories: <input type="checkbox"/> Power cord <input type="checkbox"/> Printer Cable <input checked="" type="checkbox"/> Static Bag <input type="checkbox"/> 12V DC Cable Notes: <u>Note indicating printer port loose. SLH 5/27/2025</u>	Quality Checks By <u>SLH</u> Date <u>06/02/2025</u> <input checked="" type="checkbox"/> Breath Tube Screen <input checked="" type="checkbox"/> Replace External O-Rings <input checked="" type="checkbox"/> Instrument Set Up Verified <input checked="" type="checkbox"/> R-Value <u>219</u> <input checked="" type="checkbox"/> Flow Verification (L/s) Flow Column # <u>ATP105</u> 32 mm <u>0.156</u> (.139 - .169) 36 mm <u>0.167</u> (.156 - .190) 53 mm <u>0.234</u> (.228 - .278) 103 mm <u>0.507</u> (.447 - .547) <input checked="" type="checkbox"/> Barometric Pressure Check Gauge ID # <u>28421</u> <input checked="" type="checkbox"/> Stability Checks	Flow Calibration By _____ Date _____ Flow Column # _____ <input type="checkbox"/> 5L/min – 17mm <input type="checkbox"/> 15L/min – 53mm <input type="checkbox"/> 30L/min – 103mm <input type="checkbox"/> R-Value _____ <input type="checkbox"/> Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547)																			
	<table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #/Exp</th> </tr> </thead> <tbody> <tr> <td rowspan="2">0.050</td> <td rowspan="2">MP5088</td> <td>202406K</td> </tr> <tr> <td>06/19/2026</td> </tr> <tr> <td rowspan="2">0.080</td> <td rowspan="2">MP5089</td> <td>202406L</td> </tr> <tr> <td>06/19/2026</td> </tr> <tr> <td rowspan="2">0.200</td> <td rowspan="2">MP5090</td> <td>202406N</td> </tr> <tr> <td>06/20/2026</td> </tr> <tr> <td rowspan="2">0.080 DGS</td> <td rowspan="2">N/A</td> <td>AG429602</td> </tr> <tr> <td>10/22/2026</td> </tr> </tbody> </table>	Simulator	Serial #	Lot #/Exp	0.050	MP5088	202406K	06/19/2026	0.080	MP5089	202406L	06/19/2026	0.200	MP5090	202406N	06/20/2026	0.080 DGS	N/A	AG429602	10/22/2026	Maintenance By <u>SLH</u> Date <u>06/02/2025</u> <input type="checkbox"/> Battery Replacement <input type="checkbox"/> Dry Gas Regulator Replacement <input type="checkbox"/> Breath Tube Replacement <input checked="" type="checkbox"/> Other <u>Added printer screw to fix loose printer port. SLH 6/2/2025</u>
Simulator	Serial #	Lot #/Exp																			
0.050	MP5088	202406K																			
		06/19/2026																			
0.080	MP5089	202406L																			
		06/19/2026																			
0.200	MP5090	202406N																			
		06/20/2026																			
0.080 DGS	N/A	AG429602																			
		10/22/2026																			

Calibration Adjustment By _____ Barometric Pressure Gauge _____ ID # _____ <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #</th> <th>Expiration</th> </tr> </thead> <tbody> <tr> <td>0.000</td> <td></td> <td>N/A</td> <td>N/A</td> </tr> <tr> <td>0.040</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.100</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.200</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.300</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td></td> <td></td> </tr> </tbody> </table> <input type="checkbox"/> Post Calibration Adjustment Stability Checks <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #</th> <th>Expiration</th> </tr> </thead> <tbody> <tr> <td>0.050</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.200</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td></td> <td></td> </tr> </tbody> </table>	Simulator	Serial #	Lot #	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Simulator	Serial #	Lot #	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			Department Inspection By <u>SLH</u> Barometric Pressure ID# <u>28662</u> Gauge <u>1013</u> Instrument <u>1014</u> Mouth Alcohol Solution Lot # <u>2025A</u> Acetone Stock Solution Lot # <u>2024B</u> <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> </tr> </thead> <tbody> <tr> <td>0.000</td> <td>MP5086</td> </tr> <tr> <td>Interferent</td> <td>MP5087</td> </tr> <tr> <td>0.050</td> <td>MP5088</td> </tr> <tr> <td>0.080</td> <td>MP5089</td> </tr> <tr> <td>0.200</td> <td>MP5090</td> </tr> </tbody> </table> Attachments <input checked="" type="checkbox"/> Form 41 <input checked="" type="checkbox"/> Stability Checks <input checked="" type="checkbox"/> Calibration Certificate <input type="checkbox"/> Calibration Adjustment <input type="checkbox"/> Post-Stability Checks <input type="checkbox"/> Flow Calibration <input type="checkbox"/> Form 40 <input type="checkbox"/> Other _____	Simulator	Serial Number	0.000	MP5086	Interferent	MP5087	0.050	MP5088	0.080	MP5089	0.200	MP5090
Simulator	Serial #	Lot #	Expiration																																																										
0.000		N/A	N/A																																																										
0.040																																																													
0.100																																																													
0.200																																																													
0.300																																																													
0.080 DGS	N/A																																																												
Simulator	Serial #	Lot #	Expiration																																																										
0.050																																																													
0.080																																																													
0.200																																																													
0.080 DGS	N/A																																																												
Simulator	Serial Number																																																												
0.000	MP5086																																																												
Interferent	MP5087																																																												
0.050	MP5088																																																												
0.080	MP5089																																																												
0.200	MP5090																																																												

Notes/Suggested Service: _____ _____ _____ _____ _____ _____	<input checked="" type="checkbox"/> Instrument Complies with Chapter 11D-8, FAC <input type="checkbox"/> Instrument Does Not Comply with Chapter 11D-8, FAC <input checked="" type="checkbox"/> Return to/Place into Evidentiary Use <input type="checkbox"/> Remain Out of Evidentiary Use <input checked="" type="checkbox"/> Conduct an Agency Inspection Before Evidentiary Use <div style="display: flex; justify-content: space-between;"> <div style="text-align: center;"> <small>Digitally signed by Phil Nicodemo Date: 2025.06.11 14:35:11 -0400</small> Phil Nicodemo Tech Review / Date _____ </div> <div style="text-align: center;"> <small>Digitally signed by Shayla Platt Date: 2025.06.11 21:11:24 -0400</small> Shayla Platt Admin Review / Date _____ </div> </div>
---	---

Stability Checks

Sat 6/2/2025
80-000827

DGS

Performed Root Cause Analysis	Performed Root Cause Analysis	Performed Root Cause Analysis	Performed Root Cause Analysis
<p>0.050 g/210L 0.047 to 0.053 g/210L</p> <p><input checked="" type="checkbox"/></p> <p>Performed Root Cause Analysis</p>	<p>0.080 g/210L 0.077 to 0.083 g/210L</p> <p><input checked="" type="checkbox"/></p> <p>Performed Root Cause Analysis</p>	<p>0.200 g/210L 0.194 to 0.206 g/210L</p> <p><input checked="" type="checkbox"/></p> <p>Performed Root Cause Analysis</p>	<p>DGS 0.080 g/210L 0.077 to 0.083 g/210L 50.003 g/210L of Wet</p> <p><input checked="" type="checkbox"/></p> <p>Performed Root Cause Analysis</p>
<p>MARION COUNTY SO Intoxilyzer - Alcohol Analyzer Model 8000 06/02/2025 Software: 8100.27</p> <p>Test g/210L Time</p> <p>Air Blank 0.000 15:17 Control Test 0.047 15:18 Air Blank 0.000 15:19 Control Test 0.048 15:19 Air Blank 0.000 15:10 Control Test 0.048 15:10 Air Blank 0.000 15:11 Control Test Stats Average 0.0477 Std Dev 0.0006 Rel Std Dev(%) 1.2112</p> <p><i>Messick</i> Operator's Signature</p>	<p>MARION COUNTY SO Intoxilyzer - Alcohol Analyzer Model 8000 06/02/2025 Software: 8100.27</p> <p>Test g/210L Time</p> <p>Air Blank 0.000 15:02 Control Test 0.077 15:03 Air Blank 0.000 15:03 Control Test 0.078 15:04 Air Blank 0.000 15:04 Control Test 0.078 15:05 Air Blank 0.000 15:06 Control Test Stats Average 0.0777 Std Dev 0.0006 Rel Std Dev(%) 0.7434</p> <p><i>Messick</i> Operator's Signature</p>	<p>MARION COUNTY SO Intoxilyzer - Alcohol Analyzer Model 8000 06/02/2025 Software: 8100.27</p> <p>Test g/210L Time</p> <p>Air Blank 0.000 15:13 Control Test 0.197 15:13 Air Blank 0.000 15:14 Control Test 0.198 15:15 Air Blank 0.000 15:15 Control Test 0.198 15:16 Air Blank 0.000 15:16 Control Test Stats Average 0.1977 Std Dev 0.0006 Rel Std Dev(%) 0.2921</p> <p><i>Messick</i> Operator's Signature</p>	<p>MARION COUNTY SO Intoxilyzer - Alcohol Analyzer Model 8000 06/02/2025 Software: 8100.27</p> <p>Test g/210L Time</p> <p>Air Blank 0.000 15:19 Control Test 0.079 15:19 Air Blank 0.000 15:20 Control Test 0.078 15:20 Air Blank 0.000 15:20 Control Test 0.080 15:21 Air Blank 0.000 15:21 Control Test Stats Average 0.0750 Std Dev 0.0010 Rel Std Dev(%) 1.2658</p> <p><i>Messick</i> Operator's Signature</p>

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: MARION COUNTY SO
Time of Inspection: 13:44

Date of Inspection: 06/03/2025

Serial Number: 80-000827
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202406K Exp: 06/19/2026	0.08g/210L Test (g/210L) Lot#:202406L Exp: 06/19/2026	0.20g/210L Test (g/210L) Lot#:202406N Exp: 06/20/2026	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG429602 Exp: 10/22/2026
0.000	0.047	0.077	0.197	0.079
0.000	0.048	0.077	0.198	0.078
0.000	0.047	0.078	0.197	0.079
0.000	0.048	0.077	0.198	0.078
0.000	0.048	0.077	0.198	0.078
0.000	0.047	0.077	0.198	0.078
0.000	0.047	0.077	0.198	0.078
0.000	0.047	0.078	0.198	0.078
0.000	0.047	0.077	0.198	0.079
0.000	0.048	0.077	0.198	0.078


Standard Deviations	0.0005	0.0004	0.0004	0.0004
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0004 Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.


I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



LEANDRA HIGGINBOTHAM

Signature and Printed Name

06/03/2025
Date

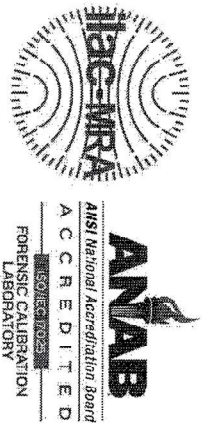

Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
2331 Phillips Road
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-000827, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-000827</u>	UNCERTAINTY* ±	
Owning Agency:	<u>MARION COUNTY SO</u>	0.050 g/210 L	0.004
Calibration Date:	<u>06/03/2025</u>	0.080 g/210 L	0.004
Calibration Time:	<u>13:44</u>	0.200 g/210 L	0.007
		0.080 g/210 L Dry Gas Control	0.005

All results are reported in g/210 L. Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration. *Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence (k=3). The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACCS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/IEC 17025 Standards. Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/IEC 17025 standards. This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

Date 06/03/2025

LEANDRA HIGGINBOTHAM,
Department Inspector