

Alcohol Testing Program - Instrument Processing Sheet

Agency: TARPON SPRINGS PD

Instrument Serial Number: 80-001065

Date In: 6/12/2026

DI Completion Date: 6/17/2026

☒ Ship ☐ P/U ☐ H/D ☐ CMI ☐ EE

Intake By: <u>WKP</u> Date: <u>6/12/2026</u>				Quality Checks By: <u>KTS</u> Date: <u>6/16/2026</u>				Flow Adjustment By: _____											
☒ Annual ☐ Dropped Off ☐ Registration ☐ Return from CMI / EE ☐ Training Instrument Visual Inspection ☒ Case ☒ Handle ☒ Keyboard ☒ Dry Gas Shelf ☒ Feet ☒ Breath Tube ☒ Ports ☒ Screws Tight Other Equipment/Accessories ☐ Power Cord ☐ Printer Cable ☐ Static Bag ☐ 12V DC Cable Notes:				☒ Breath Tube Screen ☒ Replace External O-Rings ☒ Instrument Set Up Verified ☒ R-Value: <u>190</u> ☒ Flow Verification (L/s) Flow Column #: <u>ATP102</u> 32 mm <u>0.156</u> (.139-.169) 36 mm <u>0.167</u> (.156-.190) 53 mm <u>0.234</u> (.228-.278) 103 mm <u>0.488</u> (.447-.547) ☒ Barometric Pressure Check Gauge ID #: <u>28427</u> Gauge: <u>1009</u> Instrument: <u>1009</u> ☒ Stability Checks				Flow Column #: _____ ☐ 5L/min – 17mm ☐ 15L/min – 53mm ☐ 30L/min – 103mm ☐ R-Value: _____ ☐ Post Adjustment Verification (L/S) Flow Column #: _____ 32 mm _____ (.139-.169) 36 mm _____ (.156-.190) 53 mm _____ (.228-.278) 103 mm _____ (.447-.547)											
												Simulator		Serial #		Lot#/Exp		Maintenance By: _____ Date: _____	
												0.050		MP5088		202603A 3/3/2028		☐ Battery Replacement ☐ Dry Gas Regulator Replacement	
												0.080		MP5089		202603B 3/3/2028		☐ Tank Sensor Tare ☐ Breath Tube Replacement	
												0.200		MP5090		202603D 3/4/2028		☐ Other:	
0.080 DGS		N/A		23825080A1 10/5/2027															
Optical Bench Adjustment By: _____				Department Inspection By: <u>KTS</u>															
Barometric Pressure Gauge: _____ ID#: _____				Barometric Pressure ID#: <u>28427</u>															
Simulator		Serial #		Lot #		Expiration		Gauge: <u>1009</u> Instrument: <u>1009</u>											
0.000				N/A		N/A		Mouth Alcohol Solution Lot #: <u>2025-D</u> Exp: <u>9/25/2027</u>											
0.040								Acetone Stock Solution Lot #: <u>2025-B</u> Exp: <u>9/22/2027</u>											
0.100								Simulator		Serial Number									
0.200								0.000		MP6289									
0.300								Interferent		MP5087									
0.080 DGS		N/A						0.050		MP5088									
☐ Post Optical Bench Adjustment Stability Checks								0.080		MP5089									
Simulator		Serial #		Lot #		Expiration		0.200		MP5090									
0.050								Attachments											
0.080								☒ Form 41		☐ Post-Stability Checks									
0.200								☒ Stability Checks		☐ Flow Adjustment									
0.080 DGS		N/A						☒ Calibration Certificate		☐ Form 40									
Gauge ID #: _____								☐ Optical Bench Adjustment		☐ Other:									
Gauge: _____ Instrument: _____																			
Notes/Suggested Service:				☒ Instrument Complies with Chapter 11D-8, FAC ☐ Instrument Does Not Comply with Chapter 11D-8, FAC															
				☒ Return to/Place into Evidentiary Use ☐ Remain Out of Evidentiary Use															
				☒ Conduct an Agency Inspection Before Evidentiary Use															
Wen-Chi Pierson				Digitally signed by Wen-Chi Pierson Date: 2026.06.19 15:10:10 -04'00'				LeAndra Higginbotham											
Tech Review								Admin Review											

Stability Checks

0.050 g/210L	0.080 g/210L	0.200 g/210L	DGS 0.080 g/210L
0.047 to 0.053 g/210L	0.077 to 0.083 g/210L	0.194 to 0.206 g/210L	0.077 to 0.083 g/210L
≤0.003 g/210L of Wet			≤0.003 g/210L of Wet

TARPOON SPRINGS PD
Intoxilyzer - Alcotest Analyzer
Model 8100
06/16/2026
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	11:15
Control Test	0.050	11:15
Air Blank	0.000	11:16
Control Test	0.049	11:16
Air Blank	0.000	11:17
Control Test	0.050	11:18
Air Blank	0.000	11:18
Control Test Stats		
Average	0.0497	
Std Dev	0.0006	
Rel Std Dev(%)	1.1625	

TARPOON SPRINGS PD
Intoxilyzer - Alcotest Analyzer
Model 8100
06/16/2026
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	11:19
Control Test	0.080	11:20
Air Blank	0.000	11:20
Control Test	0.080	11:21
Air Blank	0.000	11:21
Control Test	0.080	11:21
Air Blank	0.000	11:22
Control Test Stats		
Average	0.0800	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

TARPOON SPRINGS PD
Intoxilyzer - Alcotest Analyzer
Model 8100
06/16/2026
Software: 8100.27


Test	g/210L	Time
Air Blank	0.000	11:29
Control Test	0.199	11:29
Air Blank	0.000	11:30
Control Test	0.200	11:31
Air Blank	0.000	11:31
Control Test	0.200	11:32
Air Blank	0.000	11:32
Control Test Stats		
Average	0.1997	
Std Dev	0.0006	
Rel Std Dev(%)	0.2892	

TARPOON SPRINGS PD
Intoxilyzer - Alcotest Analyzer
Model 8100
06/16/2026
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	11:24
Control Test	0.080	11:25
Air Blank	0.000	11:25
Control Test	0.079	11:26
Air Blank	0.000	11:27
Control Test	0.079	11:27
Air Blank	0.000	11:28
Control Test Stats		
Average	0.0793	
Std Dev	0.0006	
Rel Std Dev(%)	0.7277	


Operator's Signature


Operator's Signature

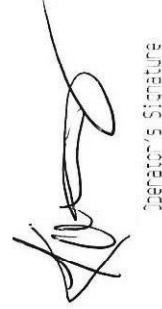
Operator's Signature


Operator's Signature

Florida Department of Law Enforcement

Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 12:51

Date of Inspection: 06/17/2026

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202603A Exp: 03/03/2028	0.08g/210L Test (g/210L) Lot#:202603B Exp: 03/03/2028	0.20g/210L Test (g/210L) Lot#:202603D Exp: 03/04/2028	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:23825080A1 Exp: 10/05/2027
0.000	0.050	0.080	0.199	0.080
0.000	0.050	0.079	0.200	0.080
0.000	0.050	0.079	0.199	0.079
0.000	0.050	0.079	0.200	0.080
0.000	0.050	0.079	0.199	0.080
0.000	0.049	0.079	0.199	0.081
0.000	0.050	0.080	0.199	0.080
0.000	0.050	0.079	0.200	0.080
0.000	0.050	0.080	0.200	0.080
0.000	0.050	0.080	0.199	0.080


Standard Deviations	0.0003	0.0005	0.0005	0.0004
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0004 Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



KATIE T SPEARIN

Signature and Printed Name

06/17/2026
Date



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
2331 Phillips Road
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-001065, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-001065</u>	UNCERTAINTY* $\pm$	
Owning Agency:	<u>TARPON SPRINGS PD</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>06/17/2026</u>	0.080 g/ 210 L	0.004
Calibration Time:	<u>12:51</u>	0.200 g/ 210 L	0.008
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.

*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ($k=3$).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/IEC 17025 standards.

This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

06/17/2026

Date

KATIE T SPEARIN,
Department Inspector

FDLE/ATP Form 69 January 2026

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality