

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD  
Time of Inspection: 19:28

Date of Inspection: 12/07/2023

Serial Number: 80-000996  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:33321080A2 Exp: 01/05/2024
0.000	0.047	0.077	0.192	0.084
0.000	0.048	0.077	0.195	0.083
0.000	0.048	0.077	0.196	0.083

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

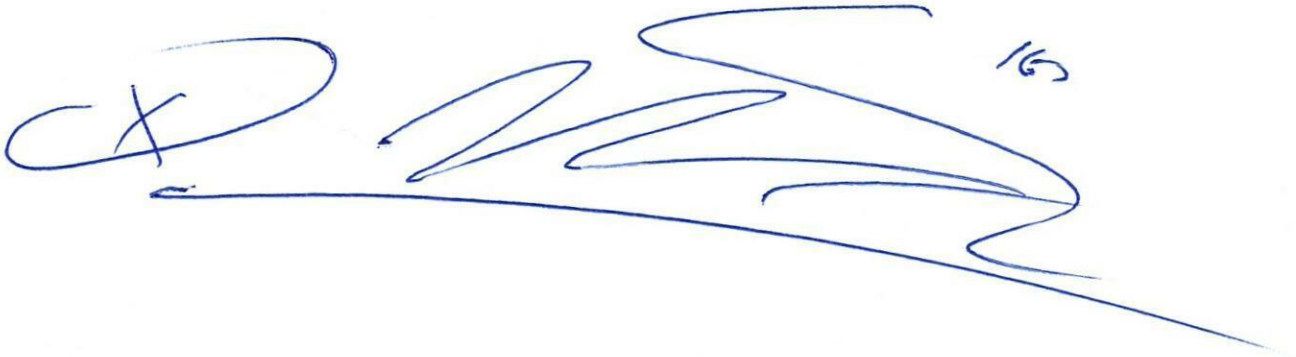

MATTHEW S RASMUSSEN  
 \_\_\_\_\_  
 Signature and Printed Name

12/07/2023  
 Date

TITUSVILLE PD  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000996  
12/07/2023  
Software: 8100.27

-----  
DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK



16

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD  
Time of Inspection: 18:42

Date of Inspection: 11/07/2023

Serial Number: 80-000996  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2014	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:33321080A2 Exp: 01/05/2024
0.000	0.047	0.078	0.193	0.083
0.000	0.048	0.078	0.196	0.083
0.000	0.048	0.078	0.197	0.083

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


167
MATTHEW S RASMUSSEN  
 \_\_\_\_\_  
 Signature and Printed Name

11/07/2023  
 Date

11-07-2023

167

TITUSVILLE PD  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000996  
11/07/2023  
Software: 8100.27

-----  
DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK



# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD  
Time of Inspection: 02:05

Date of Inspection: 09/24/2023

Serial Number: 80-000996  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:33321080A2 Exp: 01/05/2024
0.000	0.048	0.078	0.193	0.083
0.000	0.048	0.078	0.198	0.083
0.000	0.048	0.079	0.198	0.083

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


  
 MATTHEW S RASMUSSEN  
 Signature and Printed Name

09/24/2023  
 Date

TITUSVILLE PD  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000996  
09/24/2023  
Software: 8100.27

-----  
DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

(X)  167

---

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD  
Time of Inspection: 13:53

Date of Inspection: 08/29/2023

Serial Number: 80-000996  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:33321080A2 Exp: 01/05/2024
0.000	0.046	0.076	0.191	0.083
0.000	0.047	0.076	0.194	0.083
0.000	0.047	0.077	0.195	0.083


Number of Simulators Used: 5

Remarks:

A F / M A: SLOPE NOT MET FIXED DUE TO USING ENOUGH MA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 MATTHEW S RASMUSSEN  
Signature and Printed Name

08/29/2023  
Date

TITUSVILLE PD  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000996  
08/29/2023  
Software: 8100.27

-----  
DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK



# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD  
Time of Inspection: 16:30

Date of Inspection: 07/31/2023

Serial Number: 80-000996  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:33321080A2 Exp: 01/05/2024
0.000	0.046	0.076	0.190	0.079
0.000	0.047	0.076	0.194	0.079
0.000	0.047	0.076	0.195	0.079

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MATTHEW S RASMUSSEN

Signature and Printed Name

07/31/2023  
Date

TITUSVILLE PD  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000996  
07/31/2023  
Software: 8100.27

DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD

Serial Number: 80-000996

Time of Inspection: 10:45

Date of Inspection: 06/30/2023

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08g/210L Test (g/210L) Lot#: _____ Exp: _____	0.20g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: _____ Exp: _____
/ 0.000				

Number of Simulators Used: 5

**Remarks:**

00: Ambient Fail, Ambient Fail. AMBIANT FAIL TWICE DURING TESTING .


*NOTE MOUTH ALCOHOL TOO*

*CONTACTED ATP Informed  
And Inspection AGAIN  
Instructed to Perform*



The above instrument complies (     ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
Signature and Printed Name MATTHEW S RASMUSSEN

06/30/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD  
Time of Inspection: 12:23

Date of Inspection: 06/30/2023

Serial Number: 80-000996  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:33321080A2 Exp: 01/05/2024
0.000	0.041 / 0.045	0.071 / 0.076	0.170 / 0.193	0.077
0.000	0.044 / 0.046	0.075 / 0.077	0.187 / 0.196	0.077
0.000	0.045 / 0.046	0.076 / 0.076	0.193 / 0.198	0.076

Number of Simulators Used: 5

Remarks:

05: Control Outside Tolerance. 08: Control Outside Tolerance. CONTROL OUTSIDE TOL REPEATED PASSED

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MATTHEW S RASMUSSEN

Signature and Printed Name

06/30/2023  
Date



TITUSVILLE PD  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000996  
06/30/2023  
Software: 8100.27

-----  
DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD

Time of Inspection: 11:35

Date of Inspection: 05/25/2023

Serial Number: 80-000996

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:33321080A2 Exp: 01/05/2024
0.000	0.048	0.078	0.193	0.079
0.000	0.049	0.079	0.198	0.079
0.000	0.049	0.079	0.198	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MATTHEW S RASMUSSEN

Signature and Printed Name

05/25/2023  
Date

TITUSVILLE PD  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000996  
05/25/2023  
Software: 8100.27

-----  
DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD

Time of Inspection: 14:19

Date of Inspection: 04/01/2023

Serial Number: 80-000996

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:33321080A2 Exp: 01/05/2024
0.000	0.046	0.077	0.193	0.078
0.000	0.046	0.077	0.197	0.077
0.000	0.046	0.077	0.197	0.077

Number of Simulators Used: 5

**Remarks:**

A F / M A: Ambient Fail.

*Removed Mouth Alcohol Solution From Room 22 167*

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MATTHEW S RASMUSSEN

Signature and Printed Name

04/01/2023  
Date



# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD  
Time of Inspection: 13:28

Date of Inspection: 04/01/2023

Serial Number: 80-000996  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08g/210L Test (g/210L) Lot#: _____ Exp: _____	0.20g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: _____ Exp: _____

Number of Simulators Used: 5

Remarks:

Purge FAIL AFTER MOUTH ALCOHOL TEST  
"RESTARTED TEST" *MS* 167

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

*[Signature]* 167

MATTHEW S RASMUSSEN

Signature and Printed Name

04/01/2023  
Date

TITUSVILLE PD  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000996  
04/01/2023  
Software: 8100.27

-----  
DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD  
Time of Inspection: 13:28

Date of Inspection: 03/06/2023

Serial Number: 80-000996  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) <b>33321080A2</b> <del>Lot#:212054</del> Exp: 01/05/2024
0.000	0.049	0.078	0.196	0.078
0.000	0.049	0.078	0.199	0.078
0.000	0.050	0.078	0.199	0.078


Number of Simulators Used: 5

Remarks:

In correct LOT# found in Dry Gas Standard should be 33321080A2  
*MR*

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
 \_\_\_\_\_  
 Signature and Printed Name

MATTHEW S RASMUSSEN

03/06/2023  
 Date

TITUSVILLE PD  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000996  
03/06/2023  
Software: 8100.27

-----  
DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK



# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD  
Time of Inspection: 15:16

Date of Inspection: 02/17/2023

Serial Number: 80-000996  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:33321080A2 Exp: 01/05/2024
0.000 / 0.000	0.043 / 0.046	0.074 / 0.077	0.178 / 0.196	0.078
/ 0.000	0.046 / 0.046	0.077 / 0.078	0.192 / 0.197	0.079
/ 0.000	0.046 / 0.047	0.077 / 0.078	0.196 / 0.199	0.078

Number of Simulators Used: 5

**Remarks:**

00: Ambient Fail SIM NOT HOOK UP PROPERLY(. CHECKED SEAL AND TEMP (34C) . 08: Control Outside Tolerance CHECKED SEAL AND TEMP (34C) . 20: Control Outside Tolerance CHECKED SEAL AND TEMP (34C).

*MR* 02-17-2023

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

*MR* 27

MATTHEW S RASMUSSEN

Signature and Printed Name

02/17/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TITUSVILLE PD  
Time of Inspection: 13:11

Date of Inspection: 02/17/2023

Serial Number: 80-000996  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:202108D Exp: 08/17/2023
0.000	0.048	0.077	0.194	0.000 / 0.078
0.000	0.048	0.078	0.197	0.000 / 0.078
0.000	0.049	0.078	0.197	0.000 / 0.078

Number of Simulators Used: 5

**Remarks:**

08: Control Outside Tolerance SIM INSTEAD OF GAS HOSE

*Incorrect LOT And exp DATE Provided For Dry Gas Standard  
TEST to be re run ~~2~~ 02-17-2023*

The above instrument complies ( X ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MATTHEW S RASMUSSEN

Signature and Printed Name

02/17/2023  
Date

TITUSVILLE PD  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000996  
02/17/2023  
Software: 8100.27

-----  
DIAGNOSTICS

Voltage/Current Test	OK
RAM Test	OK
EEPROM Checksum Test	OK
Real Time Clock Test	OK
DSP Test	OK
Analytical Stability Test	OK
Internal Printer Test	OK
Modem Test	OK
Temperature Regulation Test	OK