

Alcohol Testing Program - Instrument Processing Sheet

Agency: HIGHLANDS COUNTY SO Instrument Serial Number: 80-007507

Date In: 6/24/2026 DI Completion Date: 7/21/26 ☒ Ship ☐ P/U ☐ H/D ☐ CMI ☐ EE

Intake By: <u>WKP</u> Date: <u>6/24/2026</u>		Quality Checks By: <u>KTS</u> Date: <u>6/25/2026</u>		Flow Adjustment By: _____																
☒ Annual ☐ Dropped Off ☐ Registration ☐ Return from CMI / EE ☐ Training Instrument Visual Inspection ☒ Case ☒ Handle ☒ Keyboard ☒ Dry Gas Shelf ☒ Feet ☒ Breath Tube ☒ Ports ☒ Screws Tight Other Equipment/Accessories ☒ Power Cord ☐ Printer Cable ☒ Static Bag ☐ 12V DC Cable Notes:		☒ Breath Tube Screen ☒ Replace External O-Rings ☒ Instrument Set Up Verified ☒ R-Value: <u>196</u> ☒ Flow Verification (L/s) Flow Column #: <u>ATP103</u> 32 mm <u>0.152</u> (.139-.169) 36 mm <u>0.164</u> (.156-.190) 53 mm <u>0.230</u> (.228-.278) 103 mm <u>0.488</u> (.447-.547) ☒ Barometric Pressure Check Gauge ID #: <u>28427</u> Gauge: <u>1012</u> Instrument: <u>1008</u> ☒ Stability Checks		Flow Column #: _____ ☐ 5L/min – 17mm ☐ 15L/min – 53mm ☐ 30L/min – 103mm ☐ R-Value: _____ ☐ Post Adjustment Verification (L/S) Flow Column #: _____ 32 mm _____ (.139-.169) 36 mm _____ (.156-.190) 53 mm _____ (.228-.278) 103 mm _____ (.447-.547)																
		<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot#/Exp</th> </tr> </thead> <tbody> <tr> <td>0.050</td> <td>MP5088</td> <td>202603A 3/3/2028</td> </tr> <tr> <td>0.080</td> <td>MP5089</td> <td>202603B 3/3/2028</td> </tr> <tr> <td>0.200</td> <td>MP5090</td> <td>202603D 3/4/2028</td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td>23825080A1 10/5/2027</td> </tr> </tbody> </table>		Simulator	Serial #	Lot#/Exp	0.050	MP5088	202603A 3/3/2028	0.080	MP5089	202603B 3/3/2028	0.200	MP5090	202603D 3/4/2028	0.080 DGS	N/A	23825080A1 10/5/2027	Maintenance By: _____ Date: _____ ☐ Battery Replacement ☐ Dry Gas Regulator Replacement ☐ Tank Sensor Tare ☐ Breath Tube Replacement ☐ Other: _____	
Simulator	Serial #	Lot#/Exp																		
0.050	MP5088	202603A 3/3/2028																		
0.080	MP5089	202603B 3/3/2028																		
0.200	MP5090	202603D 3/4/2028																		
0.080 DGS	N/A	23825080A1 10/5/2027																		
Optical Bench Adjustment By: <u>SLH</u>		Department Inspection By: <u>KTS</u>																		
Barometric Pressure Gauge: <u>1014</u> ID#: <u>28662</u>		Barometric Pressure ID#: <u>28427</u>																		
Simulator	Serial #	Lot #	Expiration	Gauge: <u>1007</u> Instrument: <u>1007</u>																
0.000	MP6294	N/A	N/A	Mouth Alcohol Solution Lot #: <u>2025-D</u> Exp: <u>9/25/27</u>																
0.040	MP6295	25090	3/11/2027	Acetone Stock Solution Lot #: <u>2025-B</u> Exp: <u>9/22/27</u>																
0.100	MP6296	24390	10/29/2026	Simulator	Serial Number															
0.200	MP6297	25020	1/14/2027	0.000	MP5086															
0.300	MP6298	25150	5/6/2027	Interferent	MP5087															
0.080 DGS	N/A	AG526603	09/23/2027	0.050	MP5088															
☒ Post Optical Bench Adjustment Stability Checks				0.080	MP5089															
Simulator	Serial #	Lot #	Expiration	0.200	MP5090															
0.050	MP5088	202603A	3/3/2028	Attachments																
0.080	MP5089	202603B	03/03/2028	☒ Form 41 ☒ Stability Checks ☒ Calibration Certificate ☒ Optical Bench Adjustment ☒ Post-Stability Checks ☐ Flow Adjustment ☐ Form 40 ☒ Other: ITP Control Test																
0.200	MP5090	202603D	3/4/2028																	
0.080 DGS	N/A	23825080A1	10/5/2027																	
Gauge ID #: <u>34419</u>																				
Gauge: <u>1014</u> Instrument: <u>1013</u>																				
Notes/Suggested Service: Post stabilities performed on 2 separate days. SLH 7/7/2026 Remaining portion of post-stabilities done on 7/15/26 by KTS. KTS 7/21/26 Tech Review: corrected spelling and added note.KTS 7/21/26 Admin Review: comment attached to document- crossed out. KTS 7/21/26				☒ Instrument Complies with Chapter 11D-8, FAC ☐ Instrument Does Not Comply with Chapter 11D-8, FAC ☒ Return to/Place into Evidentiary Use ☐ Remain Out of Evidentiary Use ☒ Conduct an Agency Inspection Before Evidentiary Use																
				Wen-Chi Pierson Digitally signed by Wen-Chi Pierson Date: 2026.07.21 09:30:58 -04'00' LeAndra Higginbotham Digitally signed by LeAndra Higginbotham Date: 2026.07.21 09:41:34 -04'00' Tech Review Admin Review																

Stability Checks

0.050 g/210L	0.080 g/210L	0.200 g/210L	DGS 0.080 g/210L																																																																																																																																																
0.047 to 0.053 g/210L	0.077 to 0.083 g/210L	0.194 to 0.206 g/210L	0.077 to 0.083 g/210L ≤ 0.003 g/210L of Wet																																																																																																																																																
HIGHLANDS COUNTY SO Intoxilyzer - Alcohol Analyzer Model 8000 06/25/2026 Software: 8100.27 <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>08:59</td></tr> <tr><td>Control Test</td><td>0.049</td><td>08:59</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:00</td></tr> <tr><td>Control Test</td><td>0.048</td><td>09:01</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:01</td></tr> <tr><td>Control Test</td><td>0.049</td><td>09:02</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:02</td></tr> <tr><td>Control Test</td><td>0.0487</td><td></td></tr> <tr><td>Average</td><td>0.0006</td><td></td></tr> <tr><td>Std Dev</td><td>1.1863</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td></td><td></td></tr> </tbody> </table>	Test	g/210L	Time	Air Blank	0.000	08:59	Control Test	0.049	08:59	Air Blank	0.000	09:00	Control Test	0.048	09:01	Air Blank	0.000	09:01	Control Test	0.049	09:02	Air Blank	0.000	09:02	Control Test	0.0487		Average	0.0006		Std Dev	1.1863		Rel Std Dev(%)			HIGHLANDS COUNTY SO Intoxilyzer - Alcohol Analyzer Model 8000 06/25/2026 Software: 8100.27 <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:03</td></tr> <tr><td>Control Test</td><td>0.077</td><td>09:04</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:04</td></tr> <tr><td>Control Test</td><td>0.078</td><td>09:05</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:06</td></tr> <tr><td>Control Test</td><td>0.077</td><td>09:06</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:07</td></tr> <tr><td>Control Test</td><td>0.0773</td><td></td></tr> <tr><td>Average</td><td>0.0006</td><td></td></tr> <tr><td>Std Dev</td><td>0.7466</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td></td><td></td></tr> </tbody> </table>	Test	g/210L	Time	Air Blank	0.000	09:03	Control Test	0.077	09:04	Air Blank	0.000	09:04	Control Test	0.078	09:05	Air Blank	0.000	09:06	Control Test	0.077	09:06	Air Blank	0.000	09:07	Control Test	0.0773		Average	0.0006		Std Dev	0.7466		Rel Std Dev(%)			HIGHLANDS COUNTY SO Intoxilyzer - Alcohol Analyzer Model 8000 06/25/2026 Software: 8100.27 <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:08</td></tr> <tr><td>Control Test</td><td>0.196</td><td>09:09</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:10</td></tr> <tr><td>Control Test</td><td>0.197</td><td>09:10</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:11</td></tr> <tr><td>Control Test</td><td>0.197</td><td>09:12</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:12</td></tr> <tr><td>Control Test</td><td>0.1967</td><td></td></tr> <tr><td>Average</td><td>0.0006</td><td></td></tr> <tr><td>Std Dev</td><td>0.2536</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td></td><td></td></tr> </tbody> </table>	Test	g/210L	Time	Air Blank	0.000	09:08	Control Test	0.196	09:09	Air Blank	0.000	09:10	Control Test	0.197	09:10	Air Blank	0.000	09:11	Control Test	0.197	09:12	Air Blank	0.000	09:12	Control Test	0.1967		Average	0.0006		Std Dev	0.2536		Rel Std Dev(%)			HIGHLANDS COUNTY SO Intoxilyzer - Alcohol Analyzer Model 8000 06/25/2026 Software: 8100.27 <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>08:53</td></tr> <tr><td>Control Test</td><td>0.081</td><td>08:54</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>08:54</td></tr> <tr><td>Control Test</td><td>0.082</td><td>08:55</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>08:55</td></tr> <tr><td>Control Test</td><td>0.081</td><td>08:55</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>08:56</td></tr> <tr><td>Control Test</td><td>0.0813</td><td></td></tr> <tr><td>Average</td><td>0.0006</td><td></td></tr> <tr><td>Std Dev</td><td>0.7099</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td></td><td></td></tr> </tbody> </table>	Test	g/210L	Time	Air Blank	0.000	08:53	Control Test	0.081	08:54	Air Blank	0.000	08:54	Control Test	0.082	08:55	Air Blank	0.000	08:55	Control Test	0.081	08:55	Air Blank	0.000	08:56	Control Test	0.0813		Average	0.0006		Std Dev	0.7099		Rel Std Dev(%)		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	08:59																																																																																																																																																	
Control Test	0.049	08:59																																																																																																																																																	
Air Blank	0.000	09:00																																																																																																																																																	
Control Test	0.048	09:01																																																																																																																																																	
Air Blank	0.000	09:01																																																																																																																																																	
Control Test	0.049	09:02																																																																																																																																																	
Air Blank	0.000	09:02																																																																																																																																																	
Control Test	0.0487																																																																																																																																																		
Average	0.0006																																																																																																																																																		
Std Dev	1.1863																																																																																																																																																		
Rel Std Dev(%)																																																																																																																																																			
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	09:03																																																																																																																																																	
Control Test	0.077	09:04																																																																																																																																																	
Air Blank	0.000	09:04																																																																																																																																																	
Control Test	0.078	09:05																																																																																																																																																	
Air Blank	0.000	09:06																																																																																																																																																	
Control Test	0.077	09:06																																																																																																																																																	
Air Blank	0.000	09:07																																																																																																																																																	
Control Test	0.0773																																																																																																																																																		
Average	0.0006																																																																																																																																																		
Std Dev	0.7466																																																																																																																																																		
Rel Std Dev(%)																																																																																																																																																			
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	09:08																																																																																																																																																	
Control Test	0.196	09:09																																																																																																																																																	
Air Blank	0.000	09:10																																																																																																																																																	
Control Test	0.197	09:10																																																																																																																																																	
Air Blank	0.000	09:11																																																																																																																																																	
Control Test	0.197	09:12																																																																																																																																																	
Air Blank	0.000	09:12																																																																																																																																																	
Control Test	0.1967																																																																																																																																																		
Average	0.0006																																																																																																																																																		
Std Dev	0.2536																																																																																																																																																		
Rel Std Dev(%)																																																																																																																																																			
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	08:53																																																																																																																																																	
Control Test	0.081	08:54																																																																																																																																																	
Air Blank	0.000	08:54																																																																																																																																																	
Control Test	0.082	08:55																																																																																																																																																	
Air Blank	0.000	08:55																																																																																																																																																	
Control Test	0.081	08:55																																																																																																																																																	
Air Blank	0.000	08:56																																																																																																																																																	
Control Test	0.0813																																																																																																																																																		
Average	0.0006																																																																																																																																																		
Std Dev	0.7099																																																																																																																																																		
Rel Std Dev(%)																																																																																																																																																			
 Operator's Signature	 Operator's Signature	 Operator's Signature	 Operator's Signature																																																																																																																																																

HIGHLANDS COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-007507
07/07/2026 13:55:49 *Sub*

Auto Calibration

pg 1 of 2

<<<<< 3um >>>>> <<<<< 9um >>>>>

Solution = 0.000 g/210L or 0.0000 mg/l, Samples = 4, Discarded = 1
Sample % Abs (% Abs Ref) % Abs (% Abs Ref)
Sample #1 0.1140 (-0.0180) 0.1050 (-0.0120)
Sample #2 0.0740 (0.0120) 0.0850 (0.0000)
Sample #3 0.1020 (0.0160) 0.0910 (-0.0060)
Sample #4 0.0900 (0.0430) 0.0790 (0.0190)
Avg % Abs 0.0887 (0.0237) 0.0850 (0.0043)
STD DEV 0.0140 (0.0169) 0.0060 (0.0131)
REL STD DEV 15.843 (71.249) 7.059 (301.181)

Solution = 0.040 g/210L or 0.1905 mg/l, Samples = 4, Discarded = 1
Sample % Abs (% Abs Ref) % Abs (% Abs Ref)
Sample #1 0.7980 (-0.0020) 1.4300 (-0.0020)
Sample #2 0.8430 (-0.0160) 1.4480 (-0.0060)
Sample #3 0.8410 (-0.0060) 1.4540 (-0.0070)
Sample #4 0.8110 (0.0160) 1.4340 (0.0000)
Avg % Abs 0.8317 (-0.0020) 1.4453 (-0.0043)
STD DEV 0.0179 (0.0164) 0.0103 (0.0038)
REL STD DEV 2.155 (818.535) 0.710 (87.368)

Solution = 0.100 g/210L or 0.4762 mg/l, Samples = 4, Discarded = 1
Sample % Abs (% Abs Ref) % Abs (% Abs Ref)
Sample #1 1.9340 (-0.0080) 3.4330 (0.0000)
Sample #2 1.9240 (0.0080) 3.4200 (0.0080)
Sample #3 1.9170 (0.0230) 3.4080 (0.0150)
Sample #4 1.9200 (0.0200) 3.4180 (0.0000)
Avg % Abs 1.9203 (0.0170) 3.4153 (0.0077)
STD DEV 0.0035 (0.0079) 0.0064 (0.0075)
REL STD DEV 0.183 (46.690) 0.188 (97.899)

Solution = 0.200 g/210L or 0.9524 mg/l, Samples = 4, Discarded = 1
Sample % Abs (% Abs Ref) % Abs (% Abs Ref)
Sample #1 3.6330 (-0.0070) 6.5530 (-0.0030)
Sample #2 3.6900 (-0.0320) 6.5880 (-0.0230)
Sample #3 3.6740 (-0.0080) 6.5570 (-0.0070)
Sample #4 3.6420 (0.0000) 6.5480 (-0.0140)
Avg % Abs 3.6687 (-0.0133) 6.5643 (-0.0147)
STD DEV 0.0244 (0.0167) 0.0210 (0.0080)
REL STD DEV 0.666 (124.900) 0.320 (54.687)

Solution = 0.300 g/210L or 1.4286 mg/l, Samples = 4, Discarded = 1
Sample % Abs (% Abs Ref) % Abs (% Abs Ref)
Sample #1 5.2910 (-0.0130) 9.4950 (0.0040)
Sample #2 5.3360 (-0.0820) 9.5190 (-0.0360)
Sample #3 5.4010 (-0.1150) 9.5480 (-0.0490)
Sample #4 5.3950 (-0.1090) 9.5430 (-0.0390)
Avg % Abs 5.3773 (-0.1020) 9.5367 (-0.0413)
STD DEV 0.0359 (0.0176) 0.0155 (0.0068)
REL STD DEV 0.668 (17.234) 0.163 (16.468)

HIGHLANDS COUNTY SO
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-007507
 07/07/2026 13:55:49

Auto Calibration

pg 2 of 2

```

<<<<<      3um      >>>>>
-----
Zero Order Coef   -234.83
First Order Coef  2557.11
Second Order Coef  26.83
  
```

```

<<<<<      9um      >>>>>
-----
                -116.54
                1379.97
                13.63
  
```

```

-----
Act      Fit      Residual
(g/210L) (g/210L) (g/210L)
0.000    -0.000    0.0002
0.040     0.040   -0.0001
0.100     0.100   -0.0003
0.200     0.200    0.0003
0.300     0.300   -0.0001
  
```

```

-----
Act      Fit      Residual
(g/210L) (g/210L) (g/210L)
0.000     0.000   -0.0000
0.040     0.040   -0.0000
0.100     0.100    0.0001
0.200     0.200   -0.0001
0.300     0.300    0.0000
  
```

```

<<<<<      3um      >>>>>
-----
Solution = 0.080 g/210L or 0.3810 mg/l, Samples = 4, Discarded = 1
Sample
Sample #1      3275.00
Sample #2      3244.00
Sample #3      3186.00
Sample #4      3259.00
Avg            3229.6667
STD DEV        38.5530
REL STD DEV     1.194
H2O adjust (mg/l*10k) 580
  
```

```


3460.00
3476.00
3475.00
3466.00
3472.3333
5.5076
0.159
337
  
```

Barometric Pressure = 1014


*****CALIBRATION SUCCESSFUL***** SW

Post Optical Bench Adjustment Stability Checks

80-007507
SNA

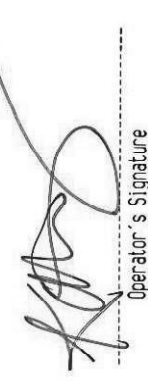0.050 g/210L	0.080 g/210L	0.200 g/210L	DGS 0.080 g/210L																																																																																																		
0.047 to 0.053 g/210L ☒	0.077 to 0.083 g/210L ☒	0.194 to 0.206 g/210L ☒	0.077 to 0.083 g/210L ☒ ≤0.003 g/210L of Wet ☒																																																																																																		
HIGHLANDS COUNTY SO Intoxilyzer - Alcohol Analyzer Model 8000 07/15/2026 Software: 8100.27 Test g/210L Time <table border="1"> <tr><td>Air Blank</td><td>0.000</td><td>12:48</td></tr> <tr><td>Control Test</td><td>0.050</td><td>12:49</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>12:49</td></tr> <tr><td>Control Test</td><td>0.049</td><td>12:50</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>12:50</td></tr> <tr><td>Control Test</td><td>0.050</td><td>12:51</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>12:52</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0497</td><td></td></tr> <tr><td>Std Dev</td><td>0.0006</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>1.1625</td><td></td></tr> </table>	Air Blank	0.000	12:48	Control Test	0.050	12:49	Air Blank	0.000	12:49	Control Test	0.049	12:50	Air Blank	0.000	12:50	Control Test	0.050	12:51	Air Blank	0.000	12:52	Control Test Stats			Average	0.0497		Std Dev	0.0006		Rel Std Dev(%)	1.1625		HIGHLANDS COUNTY SO Intoxilyzer - Alcohol Analyzer Model 8000 07/15/2026 Software: 8100.27 Test g/210L Time <table border="1"> <tr><td>Air Blank</td><td>0.000</td><td>12:40</td></tr> <tr><td>Control Test</td><td>0.196</td><td>12:41</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>12:41</td></tr> <tr><td>Control Test</td><td>0.196</td><td>12:42</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>12:43</td></tr> <tr><td>Control Test</td><td>0.197</td><td>12:43</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>12:44</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.1963</td><td></td></tr> <tr><td>Std Dev</td><td>0.0006</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>0.2941</td><td></td></tr> </table>	Air Blank	0.000	12:40	Control Test	0.196	12:41	Air Blank	0.000	12:41	Control Test	0.196	12:42	Air Blank	0.000	12:43	Control Test	0.197	12:43	Air Blank	0.000	12:44	Control Test Stats			Average	0.1963		Std Dev	0.0006		Rel Std Dev(%)	0.2941		HIGHLANDS COUNTY SO Intoxilyzer - Alcohol Analyzer Model 8000 07/07/2026 Software: 8100.27 Test g/210L Time <table border="1"> <tr><td>Air Blank</td><td>0.000</td><td>15:32</td></tr> <tr><td>Control Test</td><td>0.080</td><td>15:32</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>15:33</td></tr> <tr><td>Control Test</td><td>0.080</td><td>15:33</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>15:34</td></tr> <tr><td>Control Test</td><td>0.081</td><td>15:34</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>15:34</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0803</td><td></td></tr> <tr><td>Std Dev</td><td>0.0006</td><td></td></tr> <tr><td>Rel Std Dev(%)</td><td>0.7187</td><td></td></tr> </table>	Air Blank	0.000	15:32	Control Test	0.080	15:32	Air Blank	0.000	15:33	Control Test	0.080	15:33	Air Blank	0.000	15:34	Control Test	0.081	15:34	Air Blank	0.000	15:34	Control Test Stats			Average	0.0803		Std Dev	0.0006		Rel Std Dev(%)	0.7187	
Air Blank	0.000	12:48																																																																																																			
Control Test	0.050	12:49																																																																																																			
Air Blank	0.000	12:49																																																																																																			
Control Test	0.049	12:50																																																																																																			
Air Blank	0.000	12:50																																																																																																			
Control Test	0.050	12:51																																																																																																			
Air Blank	0.000	12:52																																																																																																			
Control Test Stats																																																																																																					
Average	0.0497																																																																																																				
Std Dev	0.0006																																																																																																				
Rel Std Dev(%)	1.1625																																																																																																				
Air Blank	0.000	12:40																																																																																																			
Control Test	0.196	12:41																																																																																																			
Air Blank	0.000	12:41																																																																																																			
Control Test	0.196	12:42																																																																																																			
Air Blank	0.000	12:43																																																																																																			
Control Test	0.197	12:43																																																																																																			
Air Blank	0.000	12:44																																																																																																			
Control Test Stats																																																																																																					
Average	0.1963																																																																																																				
Std Dev	0.0006																																																																																																				
Rel Std Dev(%)	0.2941																																																																																																				
Air Blank	0.000	15:32																																																																																																			
Control Test	0.080	15:32																																																																																																			
Air Blank	0.000	15:33																																																																																																			
Control Test	0.080	15:33																																																																																																			
Air Blank	0.000	15:34																																																																																																			
Control Test	0.081	15:34																																																																																																			
Air Blank	0.000	15:34																																																																																																			
Control Test Stats																																																																																																					
Average	0.0803																																																																																																				
Std Dev	0.0006																																																																																																				
Rel Std Dev(%)	0.7187																																																																																																				
 Operator's Signature	 Operator's Signature	 Operator's Signature	 Operator's Signature																																																																																																		

80-007507 7/15/26



HIGHLANDS COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-007507
07/15/2026
Software: 8100.27


control* KTS 7/21/26

Inadvertently hit ITP ~~control~~ test instead of stability test.
7/15/26 KTS

: ITP CONTROL TEST :

Test	g/210L	Time
Air Blank	ABT*	12:39
Air Blank	0.000	12:39

*Sequence Aborted



Operator's Signature

KTS 7/21/26

Remaining portion of post-stabilities done on 7/

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: HIGHLANDS COUNTY SO
Time of Inspection: 09:04

Date of Inspection: 07/21/2026

Serial Number: 80-007507
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202603A Exp: 03/03/2028	0.08g/210L Test (g/210L) Lot#:202603B Exp: 03/03/2028	0.20g/210L Test (g/210L) Lot#:202603D Exp: 03/04/2028	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:23825080A1 Exp: 10/05/2027
0.000	0.050	0.078	0.198	0.080
0.000	0.050	0.079	0.199	0.080
0.000	0.050	0.078	0.199	0.081
0.000	0.050	0.078	0.198	0.080
0.000	0.050	0.079	0.199	0.080
0.000	0.050	0.079	0.199	0.081
0.000	0.050	0.079	0.199	0.080
0.000	0.050	0.079	0.199	0.080
0.000	0.050	0.079	0.199	0.080
0.000	0.050	0.079	0.199	0.080

Standard Deviations	0.0000	0.0004	0.0004	0.0004
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5

Remarks:

Remaining portion of post-stabilities done 07

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

KATIE T SPEARIN

Signature and Printed Name

07/21/2026
Date



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
2331 Phillips Road
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-007507, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-007507</u>	UNCERTAINTY* $\pm$	
Owning Agency:	<u>HIGHLANDS COUNTY SO</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>07/21/2026</u>	0.080 g/ 210 L	0.004
Calibration Time:	<u>09:04</u>	0.200 g/ 210 L	0.008
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.
*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ($k=3$).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards.
This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

FDLE/ATP Form 69 January 2026
Issuing Authority: Alcohol Testing Program

07/21/2026

Date

KATIE T SPEARIN,
Department Inspector

Service • Integrity • Respect • Quality