

Alcohol Testing Program - Instrument Processing Sheet

Agency: PINELLAS COUNTY SO Instrument Serial Number: 80-001273
 Date In: 1/9/2026 DI Completion Date: 1/16/26 Ship P/U H/D CMI EE

Intake By: <u>WKP</u> Date: <u>1/9/2026</u> <input checked="" type="checkbox"/> Annual <input type="checkbox"/> Dropped Off <input type="checkbox"/> Registration <input type="checkbox"/> Return from CMI / EE <input type="checkbox"/> Training Instrument Visual Inspection <input checked="" type="checkbox"/> Case <input checked="" type="checkbox"/> Handle <input checked="" type="checkbox"/> Keyboard <input checked="" type="checkbox"/> Dry Gas Shelf <input checked="" type="checkbox"/> Feet <input checked="" type="checkbox"/> Breath Tube <input checked="" type="checkbox"/> Ports <input checked="" type="checkbox"/> Screws Tight Other Equipment/Accessories <input type="checkbox"/> Power Cord <input type="checkbox"/> Printer Cable <input type="checkbox"/> Static Bag <input type="checkbox"/> 12V DC Cable Notes:	Quality Checks By: <u>KTS</u> Date: <u>1/12/26</u> <input checked="" type="checkbox"/> Breath Tube Screen <input checked="" type="checkbox"/> Replace External O-Rings <input checked="" type="checkbox"/> Instrument Set Up Verified <input checked="" type="checkbox"/> R-Value: <u>129 / 123</u> <input checked="" type="checkbox"/> Flow Verification (L/s) Flow Column #: <u>ATP103</u> 32 mm <u>0.140 / 0.140</u> (.139-.169) 36 mm <u>0.156 / 0.156</u> (.156-.190) 53 mm <u>0.234 / 0.232</u> (.228-.278) 103 mm <u>0.500 / 0.492</u> (.447-.547) <input checked="" type="checkbox"/> Barometric Pressure Check Gauge ID #: <u>28427</u> Gauge: <u>1024</u> Instrument: <u>1019</u> <input checked="" type="checkbox"/> Stability Checks	Flow Adjustment By: _____ Flow Column #: _____ <input type="checkbox"/> 5L/min – 17mm <input type="checkbox"/> 15L/min – 53mm <input type="checkbox"/> 30L/min – 103mm <input type="checkbox"/> R-Value: _____ <input type="checkbox"/> Post Adjustment Verification (L/S) Flow Column #: _____ 32 mm _____ (.139-.169) 36 mm _____ (.156-.190) 53 mm _____ (.228-.278) 103 mm _____ (.447-.547)
---	--	--

Simulator	Serial #	Lot#/Exp	Maintenance By: <u>KTS</u> Date: <u>1/16/26</u>
0.050	MP5088	202406K 6/19/26	<input checked="" type="checkbox"/> Battery Replacement <input type="checkbox"/> Dry Gas Regulator Replacement
0.080	MP5089	202406L 6/19/26	<input type="checkbox"/> Tank Sensor Tare <input type="checkbox"/> Breath Tube Replacement
0.200	MP5090	202406N 6/20/26	<input type="checkbox"/> Other:
0.080 DGS	N/A	AG510701 4/17/27	



Optical Bench Adjustment By: _____	Department Inspection By: <u>KTS</u>
Barometric Pressure Gauge: _____ ID#: _____	Barometric Pressure ID#: <u>28427</u>

Simulator	Serial #	Lot #	Expiration	Gauge: <u>1018</u> Instrument: <u>1014</u>
0.000		N/A	N/A	Mouth Alcohol Solution Lot #: <u>2025-D</u> Exp: <u>9/25/27</u>
0.040				Acetone Stock Solution Lot #: <u>2025-B</u> Exp: <u>9/22/27</u>
Simulator	Serial Number			
0.100				
0.200				
0.300				
0.080 DGS	N/A			
		0.000		MP6289
		Interferent		MP6290
		0.050		MP5088
		0.080		MP5089
		0.200		MP5090

<input type="checkbox"/> Post Optical Bench Adjustment Stability Checks	Attachments																				
<table border="1" style="width:100%; border-collapse: collapse;"> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #</th> <th>Expiration</th> </tr> <tr> <td>0.050</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.200</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td></td> <td></td> </tr> </table> Gauge ID #: _____ Gauge: _____ Instrument: _____	Simulator	Serial #	Lot #	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			<input checked="" type="checkbox"/> Form 41 <input checked="" type="checkbox"/> Stability Checks <input checked="" type="checkbox"/> Calibration Certificate <input type="checkbox"/> Optical Bench Adjustment <input type="checkbox"/> Post-Stability Checks <input type="checkbox"/> Flow Adjustment <input type="checkbox"/> Form 40 <input type="checkbox"/> Other:
Simulator	Serial #	Lot #	Expiration																		
0.050																					
0.080																					
0.200																					
0.080 DGS	N/A																				

Notes/Suggested Service: Replaced battery then repeated flow verification and stabilities. KTS 1/16/26	<input checked="" type="checkbox"/> Instrument Complies with Chapter 11D-8, FAC <input type="checkbox"/> Instrument Does Not Comply with Chapter 11D-8, FAC <input checked="" type="checkbox"/> Return to/Place into Evidentiary Use <input type="checkbox"/> Remain Out of Evidentiary Use <input checked="" type="checkbox"/> Conduct an Agency Inspection Before Evidentiary Use				
	<table border="0" style="width:100%;"> <tr> <td style="width:50%; text-align: center;"> Digitally signed by Taylor Gutschow Date: 2026.01.23 11:31:14 -05'00' </td> <td style="width:50%; text-align: center;"> Digitally signed by Wen-Chi Pierson Date: 2026.01.26 15:12:54 -05'00' </td> </tr> <tr> <td style="text-align: center;">Taylor Gutschow</td> <td style="text-align: center;">Wen-Chi Pierson</td> </tr> </table>	Digitally signed by Taylor Gutschow Date: 2026.01.23 11:31:14 -05'00'	Digitally signed by Wen-Chi Pierson Date: 2026.01.26 15:12:54 -05'00'	Taylor Gutschow	Wen-Chi Pierson
Digitally signed by Taylor Gutschow Date: 2026.01.23 11:31:14 -05'00'	Digitally signed by Wen-Chi Pierson Date: 2026.01.26 15:12:54 -05'00'				
Taylor Gutschow	Wen-Chi Pierson				
Tech Review	Admin Review				

Stability Checks

0.050 g/210L 0.047 to 0.053 g/210L	0.080 g/210L 0.077 to 0.083 g/210L	0.200 g/210L 0.194 to 0.206 g/210L	DGS 0.080 g/210L 0.077 to 0.083 g/210L ≤0.003 g/210L of Wet																																																																																																																																																
<p>PINELLAS COUNTY SO Intoxilyzer - Alconol Analyzer Model: 8000 01/12/2026 Software: 8100.27</p> <p>SN 80-001273</p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.003</td><td>09:47</td></tr> <tr><td>Control Test</td><td>0.050</td><td>09:48</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:49</td></tr> <tr><td>Control Test</td><td>0.050</td><td>09:49</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:50</td></tr> <tr><td>Control Test</td><td>0.050</td><td>09:51</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:51</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0500</td><td></td></tr> <tr><td>Std Dev</td><td>0.0000</td><td></td></tr> <tr><td>Rel. Std Dev(%)</td><td>0.0000</td><td></td></tr> </tbody> </table> <p>Operator's Signature: </p>	Test	g/210L	Time	Air Blank	0.003	09:47	Control Test	0.050	09:48	Air Blank	0.000	09:49	Control Test	0.050	09:49	Air Blank	0.000	09:50	Control Test	0.050	09:51	Air Blank	0.000	09:51	Control Test Stats			Average	0.0500		Std Dev	0.0000		Rel. Std Dev(%)	0.0000		<p>PINELLAS COUNTY SO Intoxilyzer - Alconol Analyzer Model: 8000 01/12/2026 Software: 8100.27</p> <p>SN 80-001273</p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>09:39</td></tr> <tr><td>Control Test</td><td>0.080</td><td>09:39</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:40</td></tr> <tr><td>Control Test</td><td>0.080</td><td>09:40</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:41</td></tr> <tr><td>Control Test</td><td>0.080</td><td>09:41</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>09:42</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0800</td><td></td></tr> <tr><td>Std Dev</td><td>0.0000</td><td></td></tr> <tr><td>Rel. Std Dev(%)</td><td>0.0000</td><td></td></tr> </tbody> </table> <p>Operator's Signature: </p>	Test	g/210L	Time	Air Blank	0.000	09:39	Control Test	0.080	09:39	Air Blank	0.000	09:40	Control Test	0.080	09:40	Air Blank	0.000	09:41	Control Test	0.080	09:41	Air Blank	0.000	09:42	Control Test Stats			Average	0.0800		Std Dev	0.0000		Rel. Std Dev(%)	0.0000		<p>PINELLAS COUNTY SO Intoxilyzer - Alconol Analyzer Model: 8000 01/12/2026 Software: 8100.27</p> <p>SN 80-001273</p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>10:17</td></tr> <tr><td>Control Test</td><td>0.197</td><td>10:18</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:18</td></tr> <tr><td>Control Test</td><td>0.198</td><td>10:19</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:19</td></tr> <tr><td>Control Test</td><td>0.199</td><td>10:20</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:21</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.1980</td><td></td></tr> <tr><td>Std Dev</td><td>0.0010</td><td></td></tr> <tr><td>Rel. Std Dev(%)</td><td>0.5051</td><td></td></tr> </tbody> </table> <p>Operator's Signature: </p>	Test	g/210L	Time	Air Blank	0.000	10:17	Control Test	0.197	10:18	Air Blank	0.000	10:18	Control Test	0.198	10:19	Air Blank	0.000	10:19	Control Test	0.199	10:20	Air Blank	0.000	10:21	Control Test Stats			Average	0.1980		Std Dev	0.0010		Rel. Std Dev(%)	0.5051		<p>PINELLAS COUNTY SO Intoxilyzer - Alconol Analyzer Model: 8000 01/12/2026 Software: 8100.27</p> <p>SN 80-001273</p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr><td>Air Blank</td><td>0.000</td><td>10:12</td></tr> <tr><td>Control Test</td><td>0.077</td><td>10:13</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:13</td></tr> <tr><td>Control Test</td><td>0.079</td><td>10:14</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:15</td></tr> <tr><td>Control Test</td><td>0.079</td><td>10:15</td></tr> <tr><td>Air Blank</td><td>0.000</td><td>10:16</td></tr> <tr><td>Control Test Stats</td><td></td><td></td></tr> <tr><td>Average</td><td>0.0783</td><td></td></tr> <tr><td>Std Dev</td><td>0.0012</td><td></td></tr> <tr><td>Rel. Std Dev(%)</td><td>1.4741</td><td></td></tr> </tbody> </table> <p>Operator's Signature: </p>	Test	g/210L	Time	Air Blank	0.000	10:12	Control Test	0.077	10:13	Air Blank	0.000	10:13	Control Test	0.079	10:14	Air Blank	0.000	10:15	Control Test	0.079	10:15	Air Blank	0.000	10:16	Control Test Stats			Average	0.0783		Std Dev	0.0012		Rel. Std Dev(%)	1.4741	
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.003	09:47																																																																																																																																																	
Control Test	0.050	09:48																																																																																																																																																	
Air Blank	0.000	09:49																																																																																																																																																	
Control Test	0.050	09:49																																																																																																																																																	
Air Blank	0.000	09:50																																																																																																																																																	
Control Test	0.050	09:51																																																																																																																																																	
Air Blank	0.000	09:51																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0500																																																																																																																																																		
Std Dev	0.0000																																																																																																																																																		
Rel. Std Dev(%)	0.0000																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	09:39																																																																																																																																																	
Control Test	0.080	09:39																																																																																																																																																	
Air Blank	0.000	09:40																																																																																																																																																	
Control Test	0.080	09:40																																																																																																																																																	
Air Blank	0.000	09:41																																																																																																																																																	
Control Test	0.080	09:41																																																																																																																																																	
Air Blank	0.000	09:42																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0800																																																																																																																																																		
Std Dev	0.0000																																																																																																																																																		
Rel. Std Dev(%)	0.0000																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	10:17																																																																																																																																																	
Control Test	0.197	10:18																																																																																																																																																	
Air Blank	0.000	10:18																																																																																																																																																	
Control Test	0.198	10:19																																																																																																																																																	
Air Blank	0.000	10:19																																																																																																																																																	
Control Test	0.199	10:20																																																																																																																																																	
Air Blank	0.000	10:21																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.1980																																																																																																																																																		
Std Dev	0.0010																																																																																																																																																		
Rel. Std Dev(%)	0.5051																																																																																																																																																		
Test	g/210L	Time																																																																																																																																																	
Air Blank	0.000	10:12																																																																																																																																																	
Control Test	0.077	10:13																																																																																																																																																	
Air Blank	0.000	10:13																																																																																																																																																	
Control Test	0.079	10:14																																																																																																																																																	
Air Blank	0.000	10:15																																																																																																																																																	
Control Test	0.079	10:15																																																																																																																																																	
Air Blank	0.000	10:16																																																																																																																																																	
Control Test Stats																																																																																																																																																			
Average	0.0783																																																																																																																																																		
Std Dev	0.0012																																																																																																																																																		
Rel. Std Dev(%)	1.4741																																																																																																																																																		

PINELLAS COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001273
01/16/2026
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	10:26
Control Test	0.079	10:27
Air Blank	0.000	10:28
Control Test	0.080	10:28
Air Blank	0.000	10:29
Control Test	0.079	10:30
Air Blank	0.000	10:30
Control Test Stats		
Average	0.0793	
Std Dev	0.0006	
Rel Std Dev(%)	0.7277	



Operator's Signature

PINELLAS COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001273
01/16/2026
Software: 8100.27

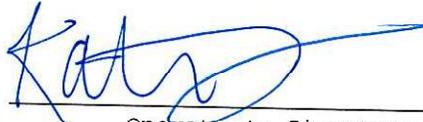
Test	g/210L	Time
Air Blank	0.000	10:22
Control Test	0.049	10:22
Air Blank	0.000	10:23
Control Test	0.049	10:24
Air Blank	0.000	10:24
Control Test	0.050	10:25
Air Blank	0.000	10:25
Control Test Stats		
Average	0.0493	
Std Dev	0.0006	
Rel Std Dev(%)	1.1703	



Operator's Signature

PINELLAS COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001273
01/16/2026
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	10:31
Control Test	0.197	10:31
Air Blank	0.000	10:32
Control Test	0.197	10:33
Air Blank	0.000	10:33
Control Test	0.197	10:34
Air Blank	0.000	10:35
Control Test Stats		
Average	0.1970	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	


Operator's Signature

PINELLAS COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001273
01/16/2026
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	10:35
Control Test	0.079	10:36
Air Blank	0.000	10:36
Control Test	0.079	10:37
Air Blank	0.000	10:37
Control Test	0.080	10:37
Air Blank	0.000	10:38
Control Test Stats		
Average	0.0793	
Std Dev	0.0006	
Rel Std Dev(%)	0.7277	



Operator's Signature

Dny

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: PINELLAS COUNTY SO
Time of Inspection: 12:10

Date of Inspection: 01/16/2026

Serial Number: 80-001273
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202406K Exp: 06/19/2026	0.08g/210L Test (g/210L) Lot#:202406L Exp: 06/19/2026	0.20g/210L Test (g/210L) Lot#:202406N Exp: 06/20/2026	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG510701 Exp: 04/17/2027
0.000	0.049	0.079	0.197	0.079
0.000	0.050	0.080	0.197	0.079
0.000	0.050	0.080	0.198	0.079
0.000	0.050	0.080	0.198	0.079
0.000	0.050	0.079	0.198	0.078
0.000	0.050	0.080	0.198	0.079
0.000	0.050	0.079	0.198	0.078
0.000	0.051	0.080	0.198	0.078
0.000	0.051	0.080	0.198	0.078
0.000	0.051	0.080	0.198	0.078
0.000	0.051	0.080	0.198	0.079


Standard Deviations	0.0006	0.0004	0.0004	0.0005
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0004 Number of Simulators Used: 5

Remarks:


The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



KATIE T SPEARIN
Signature and Printed Name

01/16/2026
Date



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
2331 Phillips Road
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-001273, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-001273</u>	UNCERTAINTY* ±
Owning Agency:	<u>PINELLAS COUNTY SO</u>	0.050 g/ 210 L 0.004
Calibration Date:	<u>01/16/2026</u>	0.080 g/ 210 L 0.004
Calibration Time:	<u>12:10</u>	0.200 g/ 210 L 0.008
		0.080 g/ 210 L Dry Gas Control 0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.

*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence (k=3).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards. This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

01/16/2026

Date

Katie Spearin
KATIE T SPEARIN,

Department Inspector

FDLE/ATP Form 69 January 2026

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality