



INSTRUMENT PROCESSING SHEET

Agency Florida Highway PatrolS/N 80-001120Florida Department of
Law EnforcementDate In 08/22/2025 DI Completion Date N/A☐ Ship ☐ P/U ☐ H/D ☒ CMI ☐ EE

Intake By <u>TDG</u> Date <u>09/24/2025</u>	Quality Checks By _____ Date _____	Flow Calibration By _____ Date _____															
☐ Annual ☐ Registration ☐ Return from CMI / EE Visual Inspection: ☒ Case ☒ Handle ☒ Keyboard ☒ Dry Gas Shelf ☒ Feet ☒ Breath Tube ☒ Ports ☒ Screws Tight Other Equipment/ Accessories: ☐ Power cord ☐ Printer Cable ☐ Static Bag ☐ 12V DC Cable Notes: <u>Missing left screw on DGS ring. Contained a note from the Agency Inspector about a failed upload. Instrument has already been calibrated this year. Added a static bag for return shipping.</u>	☐ Breath Tube Screen ☐ Replace External O-Rings ☐ Instrument Set Up Verified ☐ R-Value _____ ☐ Flow Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547) ☐ Barometric Pressure Check Gauge ID # _____ ☐ Stability Checks <table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #/Exp</th></tr></thead><tbody><tr><td>0.050</td><td></td><td></td></tr><tr><td>0.080</td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td></tr></tbody></table>	Simulator	Serial #	Lot #/Exp	0.050			0.080			0.200			0.080 DGS	N/A		Flow Column # _____ ☐ 5L/min – 17mm ☐ 15L/min – 53mm ☐ 30L/min – 103mm ☐ R-Value _____ ☐ Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547) Maintenance By <u>TDG</u> Date <u>09/24/2025</u> ☐ Battery Replacement ☐ Dry Gas Regulator Replacement ☐ Breath Tube Replacement ☒ Other <u>Replaced missing screw. Tried to upload via analog line and remote-upload across multiple days but was unsuccessful. Uploaded via direct-connect.</u>
Simulator	Serial #	Lot #/Exp															
0.050																	
0.080																	
0.200																	
0.080 DGS	N/A																

Calibration Adjustment By _____	Department Inspection By _____																																																																
Barometric Pressure Gauge _____ ID # _____ <table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.000</td><td></td><td>N/A</td><td>N/A</td></tr><tr><td>0.040</td><td></td><td></td><td></td></tr><tr><td>0.100</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.300</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table> ☐ Post Calibration Adjustment Stability Checks <table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.050</td><td></td><td></td><td></td></tr><tr><td>0.080</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table> Notes/Suggested Service: <u>Unable to upload via analog line or remote-upload. Sending to CMI. (TDG 9/30/25)</u>	Simulator	Serial #	Lot #	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Simulator	Serial #	Lot #	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			Barometric Pressure ID# _____ Gauge _____ Instrument _____ Mouth Alcohol Solution Lot # _____ Acetone Stock Solution Lot # _____ <table border="1"><thead><tr><th>Simulator</th><th>Serial Number</th></tr></thead><tbody><tr><td>0.000</td><td></td></tr><tr><td>Interferent</td><td></td></tr><tr><td>0.050</td><td></td></tr><tr><td>0.080</td><td></td></tr><tr><td>0.200</td><td></td></tr></tbody></table> Attachments <table border="1"><tbody><tr><td>☐ Form 41 ☐ Stability Checks ☐ Calibration Certificate ☐ Calibration Adjustment</td><td>☐ Post-Stability Checks ☐ Flow Calibration ☐ Form 40 ☒ Other <u>Agency Note/Form 51</u></td></tr></tbody></table> ☐ Instrument Complies with Chapter 11D-8, FAC ☐ Instrument Does Not Comply with Chapter 11D-8, FAC ☐ Return to/Place into Evidentiary Use ☒ Remain Out of Evidentiary Use ☐ Conduct an Agency Inspection Before Evidentiary Use <table border="1"><tbody><tr><td>Phil Nicodemo Digitally signed by Phil Nicodemo Date: 2025.10.08 13:05:28 -04'00'</td><td>Shayla Platt Digitally signed by Shayla Platt Date: 2025.10.15 18:44:21 -04'00'</td></tr></tbody></table> Tech Review / Date _____ Admin Review / Date _____	Simulator	Serial Number	0.000		Interferent		0.050		0.080		0.200		☐ Form 41 ☐ Stability Checks ☐ Calibration Certificate ☐ Calibration Adjustment	☐ Post-Stability Checks ☐ Flow Calibration ☐ Form 40 ☒ Other <u>Agency Note/Form 51</u>	Phil Nicodemo Digitally signed by Phil Nicodemo Date: 2025.10.08 13:05:28 -04'00'	Shayla Platt Digitally signed by Shayla Platt Date: 2025.10.15 18:44:21 -04'00'
Simulator	Serial #	Lot #	Expiration																																																														
0.000		N/A	N/A																																																														
0.040																																																																	
0.100																																																																	
0.200																																																																	
0.300																																																																	
0.080 DGS	N/A																																																																
Simulator	Serial #	Lot #	Expiration																																																														
0.050																																																																	
0.080																																																																	
0.200																																																																	
0.080 DGS	N/A																																																																
Simulator	Serial Number																																																																
0.000																																																																	
Interferent																																																																	
0.050																																																																	
0.080																																																																	
0.200																																																																	
☐ Form 41 ☐ Stability Checks ☐ Calibration Certificate ☐ Calibration Adjustment	☐ Post-Stability Checks ☐ Flow Calibration ☐ Form 40 ☒ Other <u>Agency Note/Form 51</u>																																																																
Phil Nicodemo Digitally signed by Phil Nicodemo Date: 2025.10.08 13:05:28 -04'00'	Shayla Platt Digitally signed by Shayla Platt Date: 2025.10.15 18:44:21 -04'00'																																																																

1120 needs repair

Fails during upload

"Connects, unable to upload"

80-001120

9/24/25

ML

Return Material Authorization

Ship to: ☒ CMI, Inc.

☐ Enforcement Electronics

Shipment to repair facility authorized by: Andrew Sackmann on 9/30/2025

Items Returned: Instrument ☒ Supplies ☐ Other ☐ Describe: _____

Instrument Model: Intoxilyzer 8000 Serial Number: 80-001120

Bill To Address:

Florida Highway Patrol

Attn: Andrew Sackmann

Ship to Address:

Florida Department of Law Enforcement

Fort Myers Regional Operations Center

Attn: Taylor Gutschow

4700 Terminal Drive, Suite 1

Fort Myers, FL 33907

Reason for Return:

Instrument will not upload via analog line or remote-upload. Please evaluate.

Please choose one of the following options:

- ☐ 1. I _____, authorize all repairs.
- ☐ 2. I _____, authorize repairs up to \$_____.
- ☒ 3. I require an estimate **BEFORE** any repairs will be authorized and/ or conducted.

Please contact: Name: Andrew Sackmann

Phone #: 239-293-5529 Email: AndrewSackmann@flhsmv.gov

ATP Contact Name: Taylor Gutschow ATP Email: TaylorGutschow@fdle.state.fl.us



INSTRUMENT PROCESSING SHEET

Agency FL Highway Patrol

S/N 80-001120

Florida Department of
Law Enforcement

Date In 03/10/2025 DI Completion Date 03/31/2025

☐ Ship ☒ P/U ☐ H/D ☐ CMI ☐ EE

Intake	By <u>ALL</u>	Date <u>3/11/2025</u>	Quality Checks	By <u>SLH</u>	Date <u>03/26/2025</u>	Flow Calibration	By _____	Date _____																											
☒ Annual ☐ Registration ☐ Return from CMI / EE Visual Inspection: ☒ Case ☒ Handle ☒ Keyboard ☒ Dry Gas Shelf ☒ Feet ☒ Breath Tube ☒ Ports ☒ Screws Tight Other Equipment/ Accessories: ☐ Power cord ☐ Printer Cable ☐ Static Bag ☐ 12V DC Cable Notes: <u>dropoff, no box</u>			☒ Breath Tube Screen ☒ Replace External O-Rings ☒ Instrument Set Up Verified ☒ R-Value <u>202</u> ☒ Flow Verification (L/s) Flow Column # <u>ATP103</u> 32 mm <u>0.148</u> (.139 - .169) 36 mm <u>0.167</u> (.156 - .190) 53 mm <u>0.230</u> (.228 - .278) 103 mm <u>0.503</u> (.447 - .547) ☒ Barometric Pressure Check Gauge ID # <u>28427</u> ☒ Stability Checks			Flow Column # _____ ☐ 5L/min – 17mm ☐ 15L/min – 53mm ☐ 30L/min – 103mm ☐ R-Value _____ ☐ Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547)																													
			<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #/Exp</th></tr></thead><tbody><tr><td>0.050</td><td>MP6291</td><td>202406K 06/19/2026</td></tr><tr><td>0.080</td><td>MP6292</td><td>202406L 06/19/2026</td></tr><tr><td>0.200</td><td>MP6293</td><td>202406N 06/20/2026</td></tr><tr><td>0.080 DGS</td><td>N/A</td><td>06723080A5 04/05/2025</td></tr></tbody></table>	Simulator	Serial #	Lot #/Exp	0.050	MP6291	202406K 06/19/2026	0.080	MP6292	202406L 06/19/2026	0.200	MP6293	202406N 06/20/2026	0.080 DGS	N/A	06723080A5 04/05/2025			Maintenance By _____ Date _____ ☐ Battery Replacement ☐ Dry Gas Regulator Replacement ☐ Breath Tube Replacement ☐ Other _____														
Simulator	Serial #	Lot #/Exp																																	
0.050	MP6291	202406K 06/19/2026																																	
0.080	MP6292	202406L 06/19/2026																																	
0.200	MP6293	202406N 06/20/2026																																	
0.080 DGS	N/A	06723080A5 04/05/2025																																	
Calibration Adjustment By _____			Department Inspection By <u>DA</u>																																
Barometric Pressure Gauge _____ ID # _____			Barometric Pressure ID# <u>30793</u>																																
<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.000</td><td></td><td>N/A</td><td>N/A</td></tr><tr><td>0.040</td><td></td><td></td><td></td></tr><tr><td>0.100</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.300</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table>			Simulator	Serial #	Lot #	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Gauge <u>1010</u> Instrument <u>1008</u> Mouth Alcohol Solution Lot # <u>2024-A</u> Acetone Stock Solution Lot # <u>2024-B</u>				
Simulator	Serial #	Lot #	Expiration																																
0.000		N/A	N/A																																
0.040																																			
0.100																																			
0.200																																			
0.300																																			
0.080 DGS	N/A																																		
☐ Post Calibration Adjustment Stability Checks			<table border="1"><thead><tr><th>Simulator</th><th>Serial Number</th></tr></thead><tbody><tr><td>0.000</td><td>MP5086</td></tr><tr><td>Interferent</td><td>MP5087</td></tr><tr><td>0.050</td><td>MP5088</td></tr><tr><td>0.080</td><td>MP5089</td></tr><tr><td>0.200</td><td>MP5090</td></tr></tbody></table>					Simulator	Serial Number	0.000	MP5086	Interferent	MP5087	0.050	MP5088	0.080	MP5089	0.200	MP5090																
Simulator	Serial Number																																		
0.000	MP5086																																		
Interferent	MP5087																																		
0.050	MP5088																																		
0.080	MP5089																																		
0.200	MP5090																																		
<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.050</td><td></td><td></td><td></td></tr><tr><td>0.080</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table>			Simulator	Serial #	Lot #	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			Attachments ☒ Form 41 ☒ Stability Checks ☒ Calibration Certificate ☐ Calibration Adjustment ☐ Post-Stability Checks ☐ Flow Calibration ☒ Form 40 ☐ Other _____												
Simulator	Serial #	Lot #	Expiration																																
0.050																																			
0.080																																			
0.200																																			
0.080 DGS	N/A																																		
Notes/Suggested Service: _____			☒ Instrument Complies with Chapter 11D-8, FAC ☐ Instrument Does Not Comply with Chapter 11D-8, FAC ☒ Return to/Place into Evidentiary Use ☐ Remain Out of Evidentiary Use ☒ Conduct an Agency Inspection Before Evidentiary Use																																
			Shayla Platt Digitally signed by Shayla Platt Date: 2025.04.03 14:28:28 -04'00'																																
			Phil Nicodemo Digitally signed by Phil Nicodemo Date: 2025.04.03 11:31:50 -04'00'																																
			Tech Review / Date _____ Admin Review / Date _____																																

Florida Department of Law Enforcement
Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL

Time of Inspection: 11:05

Date of Inspection: 03/26/2025

Serial Number: 80-001120

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot #: Exp:

Number of Simulators Used: _____

Remarks:

BYPASS AI COMPLIANCE NOT DETERMINED

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



LEANDRA HIGGINBOTHAM

Signature and Printed Name

03/26/2025

Date

S/N: 80-001120 3.26.2025 stability check
SUA

FL HIGHWAY PATROL
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001120
03/26/2025
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	12:54
Control Test	0.049	12:55
Air Blank	0.000	12:55
Control Test	0.049	12:56
Air Blank	0.000	12:57
Control Test	0.049	12:57
Air Blank	0.000	12:58
Control Test Stats		
Average	0.0490	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

Operator's Signature

FL HIGHWAY PATROL
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001120
03/26/2025
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	12:35
Control Test	0.199	12:36
Air Blank	0.000	12:36
Control Test	0.199	12:37
Air Blank	0.000	12:38
Control Test	0.199	12:38
Air Blank	0.000	12:39
Control Test Stats		
Average	0.1990	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

Operator's Signature

FL HIGHWAY PATROL
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001120
03/26/2025
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	12:45
Control Test	0.079	12:46
Air Blank	0.000	12:46
Control Test	0.079	12:47
Air Blank	0.000	12:48
Control Test	0.079	12:48
Air Blank	0.000	12:49
Control Test Stats		
Average	0.0790	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

Operator's Signature

(DGS)
FL HIGHWAY PATROL
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001120
03/26/2025
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	13:21
Control Test	0.080	13:21
Air Blank	0.000	13:22
Control Test	0.080	13:22
Air Blank	0.000	13:22
Control Test	0.080	13:23
Air Blank	0.000	13:23
Control Test Stats		
Average	0.0800	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

Operator's Signature

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 11:26

Date of Inspection: 03/31/2025

Serial Number: 80-001120
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202406K Exp: 06/19/2026	0.08g/210L Test (g/210L) Lot#:202406L Exp: 06/19/2026	0.20g/210L Test (g/210L) Lot#:202406N Exp: 06/20/2026	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG429602 Exp: 10/22/2026
0.000	0.048	0.078	0.199	0.079
0.000	0.048	0.078	0.199	0.079
0.000	0.049	0.078	0.199	0.079
0.000	0.048	0.079	0.199	0.079
0.000	0.049	0.078	0.199	0.079
0.000	0.049	0.079	0.198	0.079
0.000	0.049	0.079	0.199	0.079
0.000	0.049	0.079	0.198	0.079
0.000	0.049	0.079	0.199	0.079
0.000	0.049	0.079	0.198	0.079

Standard Deviations	0.0004	0.0005	0.0004	0.0000
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.


I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DESTINEE N ARMSTRONG

Signature and Printed Name

03/31/2025
Date

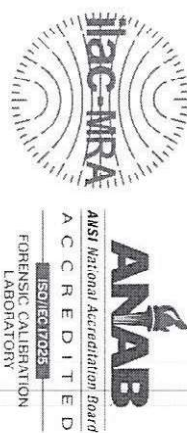

Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
2331 Phillips Road
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-001120, manufactured by CML, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-001120</u>	UNCERTAINTY * $\pm$
Owning Agency:	<u>FL HIGHWAY PATROL</u>	0.050 g/210 L 0.004
Calibration Date:	<u>03/31/2025</u>	0.080 g/210 L 0.004
Calibration Time:	<u>11:26</u>	0.200 g/210 L 0.007
		0.080 g/210 L Dry Gas Control 0.005

All results are reported in g/210 L.
Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.
*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ($k=3$).
The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION
This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/IEC 17025 standards.
This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

Date 03/31/2025 DESTINEE N ARMSTRONG,
Department Inspector
FDLE/ATP Form 69 October 2024
Issuing Authority: Alcohol Testing Program
Service • Integrity • Respect • Quality
Page 1 of 1