



INSTRUMENT PROCESSING SHEET

Agency FFWCCS/N 80-007166Florida Department of
Law EnforcementDate In 6/4/2025DI Completion Date 08/04/2025☐ Ship ☐ P/U ☐ H/D ☒ CMI ☐ EE

Intake By KTS	Date 6/4/2025	Quality Checks By KTS	Date 6/4/2025	Flow Calibration By	Date																																																																			
☒ Annual ☐ Registration ☐ Return from CMI / EE Visual Inspection: ☒ Case ☒ Handle ☒ Keyboard ☒ Dry Gas Shelf ☒ Feet ☒ Breath Tube ☒ Ports ☒ Screws Tight Other Equipment/ Accessories: ☒ Power cord ☐ Printer Cable ☒ Static Bag ☐ 12V DC Cable Notes: <u>Provided dry gas cap and regulator cap. Agency Inspector noted diagnostic fail- RTC Clock and Temp Reg fail.</u> <u>Needs battery changed. Agency Inspector also reports instrument reads 0 psi with a full DGS tank. Confirmed in lab. (TDG 6/19/25)</u>		☒ Breath Tube Screen ☒ Replace External O-Rings ☒ Instrument Set Up Verified ☒ R-Value <u>228</u> ☒ Flow Verification (L/s) Flow Column # <u>ATP106</u> 32 mm <u>0.156</u> (.139 - .169) 36 mm <u>0.167</u> (.156 - .190) 53 mm <u>0.234</u> (.228 - .278) 103 mm <u>0.496</u> (.447 - .547) ☒ Barometric Pressure Check Gauge ID # <u>28199</u> ☒ Stability Checks		Flow Column # _____ ☐ 5L/min – 17mm ☐ 15L/min – 53mm ☐ 30L/min – 103mm ☐ R-Value _____ ☐ Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547)																																																																				
		<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #/Exp</th></tr></thead><tbody><tr><td>0.050</td><td>MP8231</td><td>202406K 06/19/2026</td></tr><tr><td>0.080</td><td>MP8230</td><td>202406L 06/19/2026</td></tr><tr><td>0.200</td><td>MP8229</td><td>202406N 06/20/2026</td></tr><tr><td>0.080 DGS</td><td>N/A</td><td>AG429602 10/22/2026</td></tr></tbody></table>	Simulator	Serial #	Lot #/Exp	0.050	MP8231	202406K 06/19/2026	0.080	MP8230	202406L 06/19/2026	0.200	MP8229	202406N 06/20/2026	0.080 DGS	N/A	AG429602 10/22/2026	<table border="1"><thead><tr><th colspan="2">Maintenance By TDG</th><th>Date (See Below)</th></tr></thead><tbody><tr><td colspan="2">☒ Battery Replacement (on 6/19)</td><td></td></tr><tr><td colspan="2">☒ Dry Gas Regulator Replacement (on 7/30)</td><td></td></tr><tr><td colspan="2">☐ Breath Tube Replacement</td><td></td></tr><tr><td colspan="2">☐ Other <u>Replaced regulator and tared tank sensor on 7/30. Instrument still read 0 psi. Put old regulator back on and tared tank sensor again on 7/30.</u></td><td></td></tr></tbody></table>			Maintenance By TDG		Date (See Below)	☒ Battery Replacement (on 6/19)			☒ Dry Gas Regulator Replacement (on 7/30)			☐ Breath Tube Replacement			☐ Other <u>Replaced regulator and tared tank sensor on 7/30. Instrument still read 0 psi. Put old regulator back on and tared tank sensor again on 7/30.</u>																																							
Simulator	Serial #	Lot #/Exp																																																																						
0.050	MP8231	202406K 06/19/2026																																																																						
0.080	MP8230	202406L 06/19/2026																																																																						
0.200	MP8229	202406N 06/20/2026																																																																						
0.080 DGS	N/A	AG429602 10/22/2026																																																																						
Maintenance By TDG		Date (See Below)																																																																						
☒ Battery Replacement (on 6/19)																																																																								
☒ Dry Gas Regulator Replacement (on 7/30)																																																																								
☐ Breath Tube Replacement																																																																								
☐ Other <u>Replaced regulator and tared tank sensor on 7/30. Instrument still read 0 psi. Put old regulator back on and tared tank sensor again on 7/30.</u>																																																																								
Calibration Adjustment By _____		Department Inspection By <u>TDG</u>																																																																						
Barometric Pressure Gauge _____ ID # _____ <table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.000</td><td></td><td>N/A</td><td>N/A</td></tr><tr><td>0.040</td><td></td><td></td><td></td></tr><tr><td>0.100</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.300</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table> ☐ Post Calibration Adjustment Stability Checks <table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.050</td><td></td><td></td><td></td></tr><tr><td>0.080</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table>		Simulator	Serial #	Lot #	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Simulator	Serial #	Lot #	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			Barometric Pressure ID# <u>28199</u> Gauge <u>1017</u> Instrument <u>1014</u> Mouth Alcohol Solution Lot # <u>2024-A</u> Acetone Stock Solution Lot # <u>2023-B</u> <table border="1"><thead><tr><th>Simulator</th><th>Serial Number</th></tr></thead><tbody><tr><td>0.000</td><td>MP6284</td></tr><tr><td>Interferent</td><td>MP6285</td></tr><tr><td>0.050</td><td>MP6286</td></tr><tr><td>0.080</td><td>MP6287</td></tr><tr><td>0.200</td><td>MP6288</td></tr></tbody></table> Attachments <table border="1"><tbody><tr><td>☒ Form 41</td><td>☐ Post-Stability Checks</td></tr><tr><td>☒ Stability Checks</td><td>☐ Flow Calibration</td></tr><tr><td>☒ Calibration Certificate</td><td>☒ Form 40 (x2)</td></tr><tr><td>☐ Calibration Adjustment</td><td>☒ Other <u>Form 51</u></td></tr></tbody></table> ☒ Instrument Complies with Chapter 11D-8, FAC ☐ Instrument Does Not Comply with Chapter 11D-8, FAC ☐ Return to/Place into Evidentiary Use ☒ Remain Out of Evidentiary Use ☐ Conduct an Agency Inspection Before Evidentiary Use			Simulator	Serial Number	0.000	MP6284	Interferent	MP6285	0.050	MP6286	0.080	MP6287	0.200	MP6288	☒ Form 41	☐ Post-Stability Checks	☒ Stability Checks	☐ Flow Calibration	☒ Calibration Certificate	☒ Form 40 (x2)	☐ Calibration Adjustment	☒ Other <u>Form 51</u>
Simulator	Serial #	Lot #	Expiration																																																																					
0.000		N/A	N/A																																																																					
0.040																																																																								
0.100																																																																								
0.200																																																																								
0.300																																																																								
0.080 DGS	N/A																																																																							
Simulator	Serial #	Lot #	Expiration																																																																					
0.050																																																																								
0.080																																																																								
0.200																																																																								
0.080 DGS	N/A																																																																							
Simulator	Serial Number																																																																							
0.000	MP6284																																																																							
Interferent	MP6285																																																																							
0.050	MP6286																																																																							
0.080	MP6287																																																																							
0.200	MP6288																																																																							
☒ Form 41	☐ Post-Stability Checks																																																																							
☒ Stability Checks	☐ Flow Calibration																																																																							
☒ Calibration Certificate	☒ Form 40 (x2)																																																																							
☐ Calibration Adjustment	☒ Other <u>Form 51</u>																																																																							
Notes/Suggested Service: <u>Instrument powers on without Start Test button being pushed. (TDG 6/19/25)</u> <u>Quality Checks were performed by KTS prior to battery replacement. Instrument will be sent to CMI to evaluate 0 psi readings. Quality Checks will not be repeated due to this. (TDG 7/30/25)</u>		Phil Nicodemo Digitally signed by Phil Nicodemo Date: 2025.08.12 21:44:15 +04'00' Tech Review / Date			Shayla Platt Digitally signed by Shayla Platt Date: 2025.09.11 08:36:03 -04'00' Admin Review / Date																																																																			

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FFWCC

Time of Inspection: 15:49

Date of Inspection: 06/04/2025

Serial Number: 80-007166

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Number of Simulators Used: _____

Remarks:

Bypassed Agency Inspection to operate instrument. Compliance not determined. KTS. 6/4/25

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.




KATIE T SPEARIN

Signature and Printed Name

06/04/2025
Date

FFWCC
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-007166
06/04/2025
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	15:58
Control Test	0.048	15:58
Air Blank	0.000	15:59
Control Test	0.048	15:59
Air Blank	0.000	16:00
Control Test	0.049	16:01
Air Blank	0.000	16:01
Control Test Stats		
Average	0.0483	
Std Dev	0.0006	
Rel Std Dev(%)	1.1945	

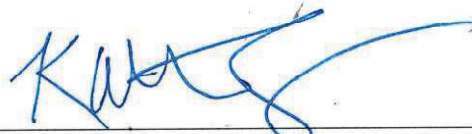

Operator's Signature

FFWCC

Intoxilyzer - Alcohol Analyzer


Model 8000

SN 80-007166

06/04/2025

Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	16:04
Control Test	0.078	16:05
Air Blank	0.000	16:05
Control Test	0.078	16:06
Air Blank	0.000	16:06
Control Test	0.078	16:07
Air Blank	0.000	16:08
Control Test Stats		
Average	0.0780	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

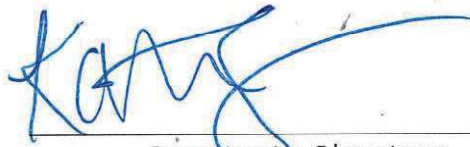
Operator's Signature

Wet

FFWCC

Intoxilyzer - Alcohol Analyzer


Model 8000

SN 80-007166

06/04/2025


Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	16:09
Control Test	0.199	16:09
Air Blank	0.000	16:10
Control Test	0.199	16:11
Air Blank	0.000	16:11
Control Test	0.197	16:12
Air Blank	0.000	16:12
Control Test Stats		
Average	0.1983	
Std Dev	0.0012	
Rel Std Dev(%)	0.5822	

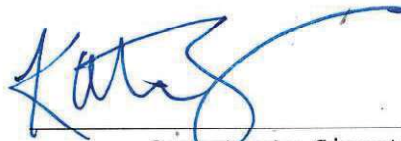
Operator's Signature

FFWCC
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-007166
06/04/2025
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	15:52
Control Test	0.078	15:52
Air Blank	0.000	15:53
Control Test	0.077	15:53
Air Blank	0.000	15:53
Control Test	0.078	15:54
Air Blank	0.000	15:54
Control Test Stats		
Average	0.0777	
Std Dev	0.0006	
Rel Std Dev(%)	0.7434	

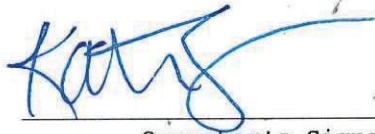

Operator's Signature

Dry

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FFWCC

Time of Inspection: 10:15

Date of Inspection: 08/04/2025

Serial Number: 80-007166

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Number of Simulators Used: _____

Remarks:

AI NOT CONDUCTED. COMPLIANCE NOT DETERMINED.

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



TAYLOR D GUTSCHOW

Signature and Printed Name

08/04/2025
Date

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: FFWCC

Time of Inspection: 15:06

Date of Inspection: 08/04/2025

Serial Number: 80-007166

Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202406K Exp: 06/19/2026	0.08g/210L Test (g/210L) Lot#:202406L Exp: 06/19/2026	0.20g/210L Test (g/210L) Lot#:202406N Exp: 06/20/2026	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG429602 Exp: 10/22/2026
0.000	0.049	0.079	0.197	0.078
0.000	0.049	0.078	0.197	0.077
0.000	0.049	0.078	0.198	0.077
0.000	0.049	0.079	0.196	0.077
0.000	0.049	0.078	0.197	0.077
0.000	0.049	0.078	0.197	0.077
0.000	0.049	0.079	0.197	0.077
0.000	0.049	0.079	0.197	0.077
0.000	0.050	0.079	0.198	0.077
0.000	0.049	0.079	0.197	0.076

Standard Deviations	0.0003	0.0005	0.0005	0.0004
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0004 Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



TAYLOR D GUTSCHOW

Signature and Printed Name

08/04/2025
Date

Return Material Authorization

Ship to: ☒ CMI, Inc.

☐ Enforcement Electronics

Shipment to repair facility authorized by: Michael Carroll on 7/30/2025

Items Returned: Instrument ☒ Supplies ☐ Other ☐ Describe: _____

Instrument Model: Intoxilyzer 8000 Serial Number: 80-007166

Bill To Address:

FFWCC

Attn: Michael Carroll

Ship to Address:

Florida Department of Law Enforcement

Fort Myers Regional Operations Center

Attn: Taylor Gutschow

4700 Terminal Drive, Suite 1

Fort Myers, FL 33907

Reason for Return:

Instrument reads 0 psi when full dry gas cylinder is attached. Also powers on without start test
button being pushed.

Please choose one of the following options:

☐ 1. I _____, authorize all repairs.

☐ 2. I _____, authorize repairs up to \$_____.

☒ 3. I require an estimate **BEFORE** any repairs will be authorized and/ or conducted.

Please contact: Name: Michael Carroll

Phone #: 850-800-7913 Email: Michael.Carroll@MyFWC.com

ATP Contact Name: Taylor Gutschow ATP Email: TaylorGutschow@fdle.state.fl.us



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
4700 Terminal Drive, Suite 1
Ft. Myers, FL 33907

This is to certify the calibration of Intoxilyzer 8000 serial number 80-007166 , manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-007166</u>	UNCERTAINTY* $\pm$	
Owning Agency:	<u>FFWCC</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>08/04/2025</u>	0.080 g/ 210 L	0.004
Calibration Time:	<u>15:06</u>	0.200 g/ 210 L	0.007
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.
*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ($k=3$).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards.
This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

Taylor
Gutschow
Digitally signed by Taylor
Gutschow
Date: 2025.08.05 15:06:32
-04'00'

08/04/2025

Date

TAYLOR D GUTSCHOW,
Department Inspector

FDLE/ATP Form 69 December 2021

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality