

Alcohol Testing Program - Instrument Processing Sheet

Agency: LAKE COUNTY SO

Instrument Serial Number: 80-006222

Date In: 7/14/2026

DI Completion Date: 7/16/2026


☒ Ship ☐ P/U ☐ H/D ☐ CMI ☐ EE

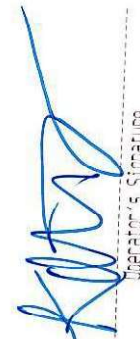
Intake By: <u>KTS</u> Date: <u>7/14/2026</u>		Quality Checks By: <u>KTS</u> Date: <u>7/16/2026</u>		Flow Adjustment By: _____																													
☒ Annual ☒ Dropped Off ☐ Registration ☐ Return from CMI / EE ☐ Training Instrument Visual Inspection ☒ Case ☒ Handle ☒ Keyboard ☒ Dry Gas Shelf ☒ Feet ☒ Breath Tube ☒ Ports ☒ Screws Tight Other Equipment/Accessories ☐ Power Cord ☐ Printer Cable ☐ Static Bag ☐ 12V DC Cable Notes: Missing both feet on dry gas shelf.		☒ Breath Tube Screen ☒ Replace External O-Rings ☒ Instrument Set Up Verified ☒ R-Value: <u>246</u> ☒ Flow Verification (L/s) Flow Column #: <u>ATP103</u> 32 mm <u>0.144</u> (.139-.169) 36 mm <u>0.160</u> (.156-.190) 53 mm <u>0.234</u> (.228-.278) 103 mm <u>0.480</u> (.447-.547) ☒ Barometric Pressure Check Gauge ID #: <u>28427</u> Gauge: <u>1013</u> Instrument: <u>1015</u> ☒ Stability Checks		Flow Column #: _____ ☐ 5L/min – 17mm ☐ 15L/min – 53mm ☐ 30L/min – 103mm ☐ R-Value: _____ ☐ Post Adjustment Verification (L/S) Flow Column #: _____ 32 mm _____ (.139-.169) 36 mm _____ (.156-.190) 53 mm _____ (.228-.278) 103 mm _____ (.447-.547)																													
						Maintenance By: _____ Date: _____																											
						☐ Battery Replacement ☐ Dry Gas Regulator Replacement ☐ Tank Sensor Tare ☐ Breath Tube Replacement ☐ Other:																											
Optical Bench Adjustment By: _____		Department Inspection By: <u>KTS</u>																															
Barometric Pressure Gauge: _____ ID#: _____		Barometric Pressure ID#: <u>28427</u>																															
<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.000</td><td></td><td>N/A</td><td>N/A</td></tr><tr><td>0.040</td><td></td><td></td><td></td></tr><tr><td>0.100</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.300</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table>		Simulator	Serial #	Lot #	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Gauge: <u>1014</u> Instrument: <u>1016</u> Mouth Alcohol Solution Lot #: <u>2025-D</u> Exp: <u>9/25/2027</u> Acetone Stock Solution Lot #: <u>2025-B</u> Exp: <u>9/22/2027</u>			
Simulator	Serial #	Lot #	Expiration																														
0.000		N/A	N/A																														
0.040																																	
0.100																																	
0.200																																	
0.300																																	
0.080 DGS	N/A																																
☐ Post Optical Bench Adjustment Stability Checks																																	
<table border="1"><thead><tr><th>Simulator</th><th>Serial #</th><th>Lot #</th><th>Expiration</th></tr></thead><tbody><tr><td>0.050</td><td></td><td></td><td></td></tr><tr><td>0.080</td><td></td><td></td><td></td></tr><tr><td>0.200</td><td></td><td></td><td></td></tr><tr><td>0.080 DGS</td><td>N/A</td><td></td><td></td></tr></tbody></table>		Simulator	Serial #	Lot #	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			Simulator		Serial Number									
Simulator	Serial #	Lot #	Expiration																														
0.050																																	
0.080																																	
0.200																																	
0.080 DGS	N/A																																
		0.000		MP5086																													
		Interferent		MP5087																													
		0.050		MP5088																													
		0.080		MP5089																													
		0.200		MP5090																													
		Attachments																															
		☒ Form 41		☐ Post-Stability Checks																													
		☒ Stability Checks		☐ Flow Adjustment																													
		☒ Calibration Certificate		☐ Form 40																													
		☐ Optical Bench Adjustment		☐ Other:																													
Gauge ID #: _____ Gauge: _____ Instrument: _____																																	
Notes/Suggested Service:		☒ Instrument Complies with Chapter 11D-8, FAC ☐ Instrument Does Not Comply with Chapter 11D-8, FAC																															
		☒ Return to/Place into Evidentiary Use ☐ Remain Out of Evidentiary Use																															
		☒ Conduct an Agency Inspection Before Evidentiary Use																															
		Wen-Chi Pierson Digitally signed by Wen-Chi Pierson Date: 2026.07.21 14:07:59 -04'00'		Taylor Gutschow Digitally signed by Taylor Gutschow Date: 2026.07.27 12:58:00 -04'00'																													
		Tech Review		Admin Review																													

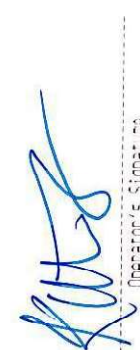
Stability Checks

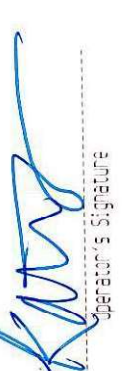
0.050 g/210L	0.080 g/210L	0.200 g/210L	DGS 0.080 g/210L
0.047 to 0.053 g/210L	0.077 to 0.083 g/210L	0.194 to 0.206 g/210L	0.077 to 0.083 g/210L
☒	☒	☒	☒
☒	☒	☒	☒

LAKE COUNTY SO				LAKE COUNTY SO				LAKE COUNTY SO				LAKE COUNTY SO			
Intoxilyzer - Alcohol Analyzer				Intoxilyzer - Alcohol Analyzer				Intoxilyzer - Alcohol Analyzer				Intoxilyzer - Alcohol Analyzer			
Model 8000				Model 8000				Model 8000				Model 8000			
07/15/2026				07/15/2026				07/15/2026				07/15/2026			
Software: 8100.27				Software: 8100.27				Software: 8100.27				Software: 8100.27			
Test	g/210L	Time		Test	g/210L	Time		Test	g/210L	Time		Test	g/210L	Time	
Air Blank	0.000	09:13		Air Blank	0.000	09:19		Air Blank	0.000	09:23		Air Blank	0.000	09:09	
Control Test	0.048	09:13		Control Test	0.078	09:19		Control Test	0.190	09:24		Control Test	0.080	09:10	
Air Blank	0.000	09:14		Air Blank	0.000	09:20		Air Blank	0.000	09:24		Air Blank	0.000	09:10	
Control Test	0.049	09:15		Control Test	0.078	09:20		Control Test	0.197	09:25		Control Test	0.079	09:11	
Air Blank	0.000	09:15		Air Blank	0.000	09:21		Air Blank	0.000	09:26		Control Test	0.079	09:11	
Control Test	0.049	09:16		Control Test	0.077	09:22		Control Test	0.198	09:26		Air Blank	0.000	09:12	
Air Blank	0.000	09:16		Air Blank	0.000	09:22		Air Blank	0.000	09:27		Control Test Stats			
Control Test Stats				Control Test Stats				Control Test Stats				Average	0.1793		
Average	0.0487			Average	0.0777			Average	0.1977			Std Dev	0.0006		
Std Dev	0.0006			Std Dev	0.0006			Std Dev	0.0006			Rel. Std Dev(%)	0.3277		
Rel. Std Dev(%)	1.1863			Rel. Std Dev(%)	0.7434			Rel. Std Dev(%)	0.2921						


Operator's Signature


Operator's Signature


Operator's Signature


Operator's Signature

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: LAKE COUNTY SO
Time of Inspection: 12:25

Date of Inspection: 07/16/2026

Serial Number: 80-006222
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202603A Exp: 03/03/2028	0.08g/210L Test (g/210L) Lot#:202603B Exp: 03/03/2028	0.20g/210L Test (g/210L) Lot#:202603D Exp: 03/04/2028	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:23825080A1 Exp: 10/05/2027
0.000	0.048	0.078	0.197	0.079
0.000	0.048	0.078	0.198	0.079
0.000	0.049	0.078	0.197	0.079
0.000	0.048	0.078	0.197	0.079
0.000	0.048	0.078	0.197	0.079
0.000	0.048	0.078	0.198	0.079
0.000	0.048	0.078	0.197	0.079
0.000	0.048	0.078	0.197	0.079
0.000	0.048	0.078	0.197	0.079
0.000	0.049	0.079	0.197	0.079
0.000	0.048	0.078	0.197	0.079


Standard Deviations	0.0004	0.0003	0.0004	0.0000
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0002 Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



KATIE T SPEARIN
Signature and Printed Name

07/16/2026
Date



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
2331 Phillips Road
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-006222, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-006222</u>	Serial Number:	<u>80-006222</u>
Owning Agency:	<u>LAKE COUNTY SO</u>	UNCERTAINTY* $\pm$	0.004
Calibration Date:	<u>07/16/2026</u>		0.004
Calibration Time:	<u>12:25</u>		0.008
			0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.

*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ($k=3$).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards.

This document shall not be reproduced except in full,

without written approval of the Florida Department of

Law Enforcement Alcohol Testing Program.

07/16/2026

Date

KATIE T SPEARIN,

Department Inspector

FDLE/ATP Form 69 January 2026

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality